



Receipt number	632-06-S-4739
Study number	14739

FINAL REPORT

Biodegradation study of 13F-SFMA by microorganisms

February 1, 2007

Kurume Laboratory
Chemicals Evaluation and Research Institute, Japan

STATEMENT

Kurume Laboratory
Chemicals Evaluation and
Research Institute, Japan

Sponsor DAIKIN INDUSTRIES, LTD.

Title Biodegradation study of 13F-SFMA by microorganisms

Study number 14739

I, the undersigned, hereby declare that this report provides a correct English translation of the Final Report (Study No. 14739, issued on February 1, 2007).

Date

August 28, 2009

Translator

GLP STATEMENT

Kurume Laboratory
Chemicals Evaluation and
Research Institute, Japan

Sponsor DAIKIN INDUSTRIES, LTD.

Title Biodegradation study of 13F-SFMA by microorganisms

Study number 14739

The study described in this report was conducted in compliance with the following GLP principles:

- (1) "Standard Concerning Testing Facility Relating to New Chemical Substances" (November 21, 2003; No. 1121003, Pharmaceutical and Food Safety Bureau, Ministry of Health, Labour and Welfare; November 17, 2003, No. 3, Manufacturing Industries Bureau, Ministry of Economy, Trade and Industry; No. 031121004, Environmental Policy Bureau, Ministry of the Environment)
- (2) "OECD Principles of Good Laboratory Practice (November 26, 1997, ENV/MC/CHEM (98)17)"

This final report reflects the raw data accurately and it has been confirmed that the test data are valid.

Date

February 1, 2007

Study Director

Signed in original
—

QUALITY ASSURANCE STATEMENT

Kurume Laboratory
Chemicals Evaluation and
Research Institute, Japan

Sponsor DAIKIN INDUSTRIES, LTD.

Title Biodegradation study of 13F-SFMA by microorganisms

Study number 14739

I assure that the final report accurately describes the test methods and procedures, and that the reported results accurately reflect the raw data of the study.

The inspections and audits of this study were carried out and the results were reported to the Study Director and the Test Facility Management by Quality Assurance Unit as follows.

Item of inspection / audit	Date of inspection / audit	Date of report to Study Director and Test Facility Management
Study plan draft	November 17, 2006	November 17, 2006
Study plan	November 20, 2006	November 20, 2006
Amendment to study plan	December 6, 2006	December 6, 2006
	December 13, 2006	December 13, 2006
	January 15, 2007	January 15, 2007
At the start of cultivation	December 13, 2006	December 13, 2006
At the middle of cultivation	December 28, 2006	December 28, 2006
At the end of cultivation	January 10, 2007	January 11, 2007
	January 11, 2007	January 11, 2007
	January 15, 2007	January 17, 2007
Raw data and final report draft	January 31, 2007	January 31, 2007
Final report	February 1, 2007	February 1, 2007

Date February 1, 2007

Head of Quality Assurance Unit Signed in original

CONTENTS

	page
Title	1
Sponsor	1
Test facility	1
Objective	1
Test method	1
Applied GLP	2
Dates	2
Storage of test item, raw data, etc.	2
Personnel	3
Approval of final report	3
SUMMARY	4
1. Test item	5
2. Test sample	5
3. Activated sludge	6
4. Performance of biodegradation test	8
5. Validity of test conditions	17
6. Factors that affected reliability of test	18
7. Results	18
8. Remarks	22

Contents of tables and figures

Contents of tables

Table-1	Calculation table for percentage biodegradation by BOD
Table-2	Calculation table for recovery rate of test item
Table-3	Calculation table for recovery rate of 13F-EtOH
Table-4	Calculation table for recovery rate of 13F-AcOH
Table-5	Calculation table for percentage biodegradation of test item
Table-6	Calculation table for percentage production of 13F-EtOH
Table-7	Calculation table for percentage production of 13F-AcOH
Table-8	Calculation table for percentage production of methacrylic acid (test solution for analysis of methacrylic acid)
Reference 1	Calculation table for percentage detection of methacrylic acid (CO ₂ absorbent, test solution for analysis of methacrylic acid)
Reference 2	Calculation table for percentage detection of methacrylic acid (CO ₂ absorbent)

Contents of figures

Fig. 1	Chart of BOD
Fig. 2-1	Chromatograms of GC analysis for calibration curve (test item)
Fig. 2-2	Calibration curve of test item
Fig. 3-1	Chromatograms of GC analysis for calibration curve (13F-EtOH)
Fig. 3-2	Calibration curve of 13F-EtOH
Fig. 4-1	Total ion chromatograms of LC-MS analysis for calibration curve (13F-AcOH)
Fig. 4-2	Calibration curve of 13F-AcOH
Fig. 5-1	Chromatograms of HPLC analysis for calibration curve (methacrylic acid)
Fig. 5-2	Calibration curve of methacrylic acid
Fig. 6	Chromatograms of GC analysis for recovery test (test item)
Fig. 7	Chromatograms of GC analysis for recovery test (13F-EtOH)
Fig. 8	Total ion chromatograms of LC-MS analysis for recovery test (13F-AcOH)
Fig. 9	Chromatograms of GC analysis for test solution (test item and 13F-EtOH)
Fig. 10	Total ion chromatograms of LC-MS analysis for test solution (13F-AcOH)
Fig. 11	Chromatograms of HPLC analysis for test solution for analysis of methacrylic acid (methacrylic acid)
Fig. 12	UV spectrum of methacrylic acid
Fig. 13	Mass spectrum of 13F-AcOH
Fig. 14-1	IR spectrum of test item measured before experimental start
Fig. 14-2	IR spectrum of test item measured after experimental completion
Reference 3	IR spectrum supplied by sponsor
Reference 4	Chromatograms of HPLC analysis for CO ₂ absorbent (methacrylic acid, test solution for analysis of methacrylic acid)
Reference 5	Chromatograms of HPLC analysis for CO ₂ absorbent (methacrylic acid)

Title

Biodegradation study of 13F-SFMA by microorganisms

Sponsor

DAIKIN INDUSTRIES, LTD.
1-1, Nishi-Hitotsuya, Settsu-shi, Osaka 566-8585, Japan

Test facility

Kurume Laboratory
Chemicals Evaluation and Research Institute, Japan
2-7, 3-chome, Miyanojin, Kurume-shi, Fukuoka 839-0801, Japan

Objective

This study was performed to evaluate the biodegradability of 13F-SFMA by microorganisms.

Test method

This study was performed according to the following test methods.

- (1) "Method for Testing the Biodegradability of Chemical Substances by Microorganisms" stipulated in the "Testing Methods for New Chemical Substances" (November 21, 2003; No. 1121002, Pharmaceutical and Food Safety Bureau, Ministry of Health, Labour and Welfare; November 13, 2003, No. 2, Manufacturing Industries Bureau, Ministry of Economy, Trade and Industry; No. 031121002, Environmental Policy Bureau, Ministry of the Environment)
- (2) "Ready Biodegradability: Modified MITI Test (I) (Guideline 301C, Revised July 17, 1992)" in the OECD Guidelines for Testing of Chemicals

Applied GLP

This study was conducted in compliance with the following GLP principles:

- (1) "Standard Concerning Testing Facility Relating to New Chemical Substances" (November 21, 2003; No. 1121003, Pharmaceutical and Food Safety Bureau, Ministry of Health, Labour and Welfare; November 17, 2003, No. 3, Manufacturing Industries Bureau, Ministry of Economy, Trade and Industry; No. 031121004, Environmental Policy Bureau, Ministry of the Environment)
- (2) "OECD Principles of Good Laboratory Practice (November 26, 1997, ENV/MC/CHEM (98)17)"

Dates

Study initiation date	November 20, 2006
Experimental starting date	December 13, 2006
Experimental completion date	January 10, 2007
Study completion date	February 1, 2007

Storage of test item, raw data, etc.

(1) Test item

The test sample is sealed in a storage vessel and stored in archives in this laboratory for ten years after the receipt of notice specified under Clause 1 or Clause 2 in Article 4, Clause 2 or Clause 3 or Clause 8 in Article 4-2, and Clause 2 in Article 5-4 or Clause 2 in Article 24 or Clause 2 in Article 25-3 of "Law Concerning Examination and Regulation of Manufacture, etc. of Chemical Substances". If it is not stable for the storage period, it is stored as long while it is kept stable. Treatment of the test sample after the storage period will be discussed with sponsor.

(2) Raw data and materials, etc.

Raw data, the study plan, documents concerning the study presented by the sponsor, the final report and necessary materials are stored in archives in this laboratory for ten years after the receipt of the notice specified under Clause 1 or Clause 2 in Article 4, Clause 2 or Clause 3 or Clause 8 in Article 4-2, and Clause 2 in Article 5-4 or Clause 2 in Article 24 or Clause 2 in Article 25-3 of "Law Concerning Examination and Regulation of Manufacture, etc. of Chemical Substances". Treatment of raw data and materials, etc. after the storage period will be discussed with sponsor.

Personnel

Study Director

(1st Chemical Safety Section)Study personnel
(Operation of biodegradation test)

Staff for cultivation of activated sludge

Approval of final report

Study Director

Date February 1, 2007

Signature Signed in original

SUMMARY

Title

Biodegradation study of 13F-SFMA by microorganisms

Conditions of cultivation

(1) Concentration of test item	100 mg/L
(2) Concentration of activated sludge (as the concentration of suspended solid)	30 mg/L
(3) Volume of test solution	300 mL
(4) Cultivation temperature	25±1 °C
(5) Cultivation duration (under the conditions of darkness)	28 days

Measurement and analysis for calculation of percentage biodegradation

- (1) Measurement of biochemical oxygen demand (BOD) with a closed system oxygen consumption measuring apparatus
- (2) Determination of test item by gas chromatography (GC)

Other analysis

- (1) Determination of 2-(perfluorohexyl)ethanol by gas chromatography (GC)
- (2) Determination of 3,3,4,4,5,5,6,6,7,7,8,8,8-tridecafluorooctanoic acid by liquid chromatography-mass spectrometry (LC-MS)
- (3) Determination of methacrylic acid by high-performance liquid chromatography (HPLC)

Results

(1) Percentage biodegradation by BOD	16%,	11%,	14%	average	14%
(2) Percentage biodegradation of test item (GC)	5%,	15%,	4%	average	8%

Conclusion

Some of the test item was converted into methacrylic acid, 2-(perfluorohexyl)ethanol and 3,3,4,4,5,5,6,6,7,7,8,8,8-tridecafluorooctanoic acid under the test conditions of this study. It was considered that some of methacrylic acid transferred from the test solution to the absorbent for carbon dioxide attached to the test vessel and that the other was biodegraded by microorganisms. The rest of the test item, 2-(perfluorohexyl)ethanol and 3,3,4,4,5,5,6,6,7,7,8,8,8-tridecafluorooctanoic acid remained in the test solution.

1. Test item


In this report, 13F-SFMA has the following chemical name, etc.

1.1 Chemical name^{*1}

3,3,4,4,5,5,6,6,7,7,8,8,8-tridecafluorooctyl methacrylate

1.2 Chemical structure, etc. ^{*1}

Structural formula

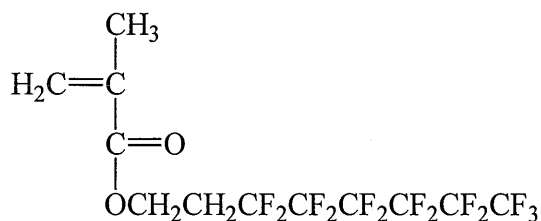

Molecular formula $\text{C}_{12}\text{H}_9\text{F}_{13}\text{O}_2$

Molecular weight 432.18

CAS number 2144-53-8

^{*1} Information supplied by the sponsor

2. Test sample

2.1 Supplier and lot number^{*1}

Supplier	DAIKIN INDUSTRIES, LTD.
Lot number	6Y002

2.2 Purity^{*1}

Test item	99.8%
Impurity	Unknown 0.2%

The test item was treated as 100% in purity.

2.3 Confirmation of test item

Two infrared (IR) spectra of the test item provided by the sponsor and measured at this laboratory were confirmed to be identical (see Fig. 14 and Reference 3).

2.4 Physicochemical properties^{*1}

Appearance	Colorless transparent liquid	
Boiling point	92°C (8 mmHg)	
Density	1.496 g/cm ³ (25°C)	
Solubility	Water	Insoluble
	Dimethylsulfoxide	Soluble (miscible in all proportions)
	Acetone	Soluble (miscible in all proportions)

^{*1} Information supplied by the sponsor

2.5 Storage and stability

Storage condition

Dark storage place at room temperature

Stability

The test item was stable under the storage conditions, as shown by the finding that IR spectra of the test item before the experimental start and after the experimental completion were identical (see Fig. 14).

3. Activated sludge

3.1 Preparation of activated sludge

Activated sludge used in the present test was prepared as follows.

(1) Sampling sites

On-site sludge sampling was carried out at the following ten locations in Japan.

Fushikogawa city sewage plant (Sapporo-shi, Hokkaido)
 Fukashiba industrial sewage plant (Kamisu-shi, Ibaraki)
 Nakahama city sewage plant (Osaka-shi, Osaka)
 Ochiai city sewage plant (Shinjuku-ku, Tokyo)
 Kitakami River (Ishinomaki-shi, Miyagi)
 Shinano River (Niigata-shi, Niigata)
 Yoshino River (Tokushima-shi, Tokushima)
 Lake Biwa (Otsu-shi, Shiga)
 Hiroshima Bay (Hiroshima-shi, Hiroshima)
 Dokai Bay (Kitakyushu-shi, Fukuoka)

(2) Sampling method

Sewage plant

Return sludge was collected.

Rivers, lake and sea

Surface water and surface soil which was in contact with the atmosphere were collected.

(3) Sampling date

September, 2006

(4) Preparation method of activated sludge

Activated sludge was prepared as follows to maintain its uniformity.

The mixed filtrate (5 L) of the supernatant of the sludge collected at sampling sites was mixed with the filtrate (5 L) of the supernatant of the activated sludge^{*2} previously cultivated for about 3 months. The mixed filtrate (10 L) was aerated^{*3} after the pH value of the mixture was adjusted to 7.0 ± 1.0 .

*2 Activated sludge cultivated the mixed filtrate (10 L) of the supernatant of the sludge collected at sampling sites according to Section 3.2.

*3 Prefiltered open air was used.

3.2 Cultivation

After ceasing aeration of the sludge mixture for approximately 30 minutes, supernatant corresponding to about one third of the whole volume was removed. Dechlorinated water was added to the remaining portion so that the total volume reached 10 L. This mixture was aerated for 30 minutes or more, and then a predetermined amount of synthetic sewage^{*4} was added to the mixture so that the concentration of the synthetic sewage was 0.1 % in the volume of dechlorinated water added. This procedure was repeated once every day. Cultivation was carried out at 25 ± 2 °C.

*4 Synthetic sewage was prepared as follows:

Glucose, peptone and potassium dihydrogenphosphate were dissolved in purified water to obtain 50 g/L of the solution for each component. The pH of the solution was adjusted to 7.0 ± 1.0 with sodium hydroxide.

3.3 Control and use

During cultivation, the appearance of the supernatant, sedimentation of the sludge, formation of flock, pH, dissolved oxygen concentration in the solution and temperature were checked to maintain a normal state of sludge. It was confirmed that these were within the scope of the control standard stipulated in the "Testing Methods for New Chemical Substances", and these results were stored as raw data. Microflora in the activated sludge was microscopically observed and sludge with no abnormal symptoms was used for the test. The activated sludge, which was cultivated for 21 hours after it had been added the synthetic sewage, was used.

3.4 Inspection of activity and date of initiation of use of activated sludge

(1) Inspection of activity

Activity of the sludge was assessed using standard items before initiation of use.

(2) Date of initiation of use

October 17, 2006

4. Performance of biodegradation test

4.1 Preparations for test

(1) Measurement of concentration of suspended solid in activated sludge

The concentration of suspended solid was measured to determine the amount of activated sludge to add.

Method	In accordance with Japanese Industrial Standards (JIS) K 0102-1998 Section 14.1
Date	December 11, 2006
Result	Concentration of suspended solid in the activated sludge was 3210 mg/L.

(2) Preparation of basal culture medium

Each 3 mL of solutions A, B, C and D, which are prescribed in JIS K 0102-1998 Section 21, were made up to 1000 mL with purified water (Japanese Pharmacopeia, Takasugi Pharmaceutical Co., Ltd.), and then the pH of this solution was adjusted to 7.0.

(3) Reference item

Aniline (reagent grade, Showa Chemicals Co., Ltd. Lot No. SR-2626U) was used as a reference item to confirm that the sludge was sufficiently active.

4.2 Preparation of test solutions

The following test solutions were prepared and cultivated under the conditions described in Section 4.3.

(1) Addition of test item or aniline

(a) Test solution (water + test item) (n=1, Vessel No. 1)

In one test vessel, 20.5 μL [$30.7 \text{ mg} = 20.5 \mu\text{L} \times 1.496 \text{ g/cm}^3$ (density)] of the test sample was taken out by microsyringe and added to 300 mL of purified water, so that the concentration of the test item reached 100 mg/L.

(b) Test solution (sludge + test item) (n=3, Vessel Nos. 2, 3 and 4)

In each test vessel, 20.5 μL [$30.7 \text{ mg} = 20.5 \mu\text{L} \times 1.496 \text{ g/cm}^3$ (density)] of the test sample was taken out by microsyringe and added to the basal culture medium [the volume was less than 300 mL by the volume (2.80 mL) of activated sludge inoculated], so that the concentration of the test item reached 100 mg/L.

(c) Test solution (sludge + aniline) (n=1, Vessel No. 6)

In one test vessel, 29.5 μL [$30 \text{ mg} = 29.5 \mu\text{L} \times 1.022 \text{ g/cm}^3$ (density)] of aniline was taken out by microsyringe and added to the basal culture medium [the volume was less than 300 mL by the volume (2.80 mL) of activated sludge inoculated], so that the concentration of aniline reached 100 mg/L.

(d) Test solution (control blank) (n=1, Vessel No. 5)

In one test vessel, nothing was added to the basal culture medium [the volume was less than 300 mL by the volume (2.80 mL) of activated sludge inoculated].

(2) Inoculation of activated sludge

The activated sludge cultivated under the conditions described in Section 3 was added to each test vessel, (b), (c) and (d), so that the concentration of the suspended solid reached 30 mg/L.

4.3 Instruments and conditions of cultivation

(1) Instruments for cultivation

Closed system oxygen consumption measuring apparatus

(Temperature controlled bath and measuring unit :

Ohkura Electric Co., Ltd.)

(Data sampler : Asahi Techneion Co., Ltd.)

Vessel 300 mL in volume

Test solutions described in Section 4.2 (a), (b) and (d)

: Improved type for volatile substance

Test solution described in Section 4.2 (c)

: Improved type

Absorbent for carbon dioxide

Soda lime No.1 (for absorption of carbon dioxide,

Wako Pure Chemical Industries, Ltd.)

The test vessels described in Section 4.2 (a), (b) and (d) were connected to the measuring unit via tube with cock.

(2) Conditions of cultivation

Cultivation temperature 25±1°C

Cultivation duration 28 days (under the conditions of darkness)

Stirring method Each test solution was stirred by a magnetic stirrer.

(3) Room

Apparatus room A

4.4 Observation and measurement of test conditions

(1) Observation of test solution

During the cultivation, the appearance of the test solution was observed once a day and conditions of the instruments were checked properly.

(2) Measurement of biochemical oxygen demand (BOD)

During the cultivation period, the change in BOD of the test solutions was measured by autorecording using a data sampler. Cultivation temperature was measured and recorded once a day.


4.5 Analysis of test solution

After the end of the cultivation, the test item and 2-(perfluorohexyl)ethanol (hereinafter referred to as 13F-EtOH), which was expected from results of the preliminary test prior to this study, in the test solutions were determined. Moreover, 3,3,4,4,5,5,6,6,7,7,8,8,8-tridecafluorooctanoic acid (hereinafter referred to as 13F-AcOH), which was also expected to be produced, in the test solutions was determined. The pH of the test solutions was not measured because the test item was thought to be a volatile compound.

Methacrylic acid [METI number (2)-1025, ready biodegradability] was expected to be produced simultaneously with the production of 13F-EtOH, in the test solutions. However, the loss of the test item and 13F-EtOH due to their volatilization in the pretreatment for analysis of methacrylic acid was considered. Therefore, additional test solutions were prepared besides the test solutions described in Section 4.2 and were used for the determination of methacrylic acid (see. Section 4.6).

4.5.1 Pretreatment of test solutions for analysis

After the end of the cultivation, the test solution (water + test item), the test solutions (sludge + test item) and the test solution (control blank) were pretreated to prepare samples for gas chromatography (GC) analysis of the test item and 13F-EtOH, and liquid chromatography-mass spectrometry (LC-MS) of 13F-AcOH as follows.

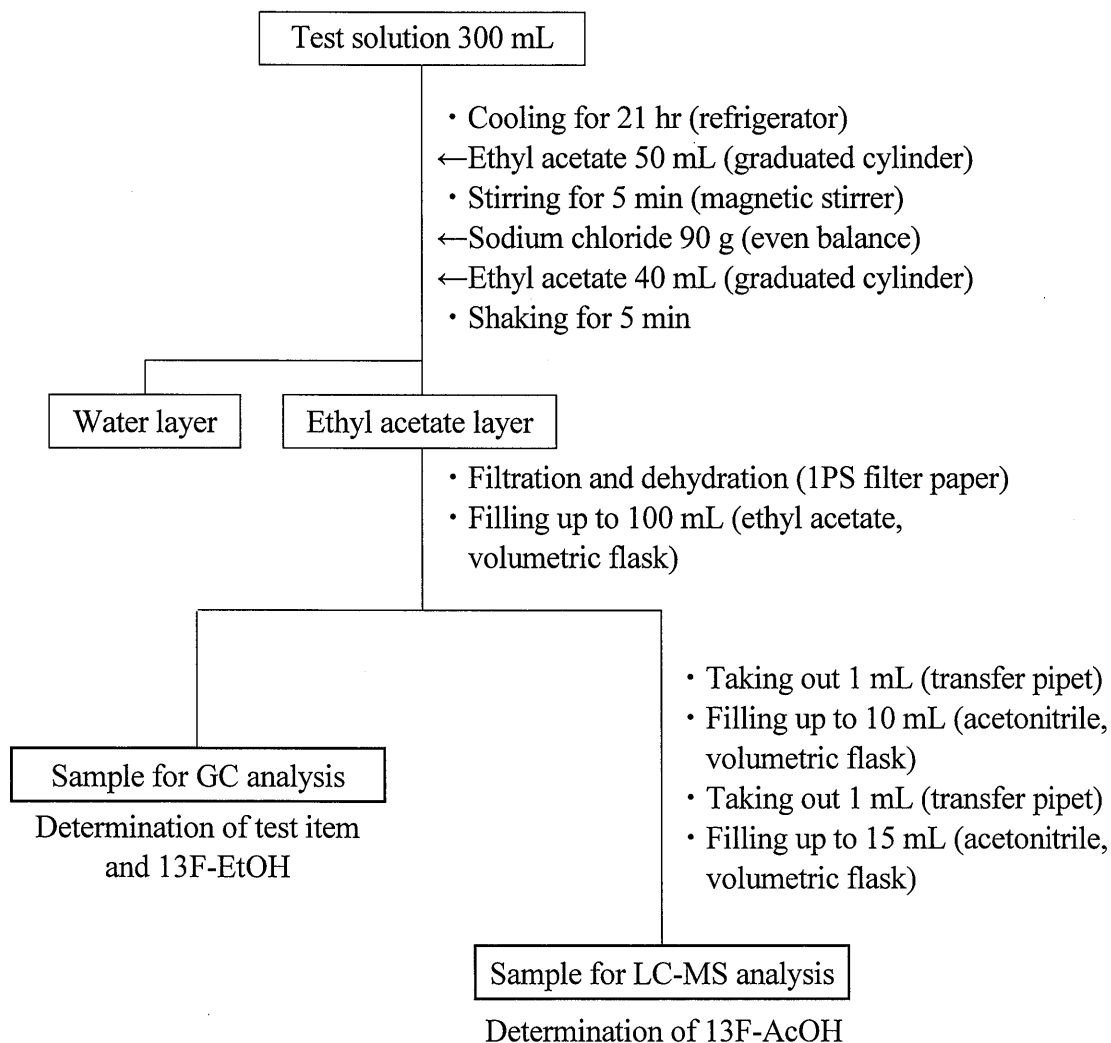

4.5.2 Quantitative analysis

(1) Determinations of test item and 13F-EtOH

The samples for GC analysis were analyzed under the following conditions. The concentration of the test item in the sample for GC analysis was proportionally calculated by comparing the peak area on the chromatogram of the sample for GC analysis with that on the chromatogram of 307 mg/L standard solution (see Table-5 and Fig. 9). The concentration of 13F-EtOH in the sample for GC analysis was proportionally calculated by comparing the peak area on the chromatogram of the sample for GC analysis with that on the chromatogram of 252 mg/L standard solution (see Table-6 and Fig. 9).

The lowest detectable peak area of the test item and 13F-EtOH was regarded as $1800 \mu\text{V} \cdot \text{sec}$ considering the noise level, which corresponded to the test item concentration of 3.0 mg/L and 13F-EtOH concentration of 4.3 mg/L.

(a) Analytical conditions

Instrument	Gas chromatograph Hewlett-Packard Company type HP6890 Series
Detector	Flame ionization detector (FID)
Column	DB-17 film thickness 0.25 μm (Agilent Technologies, Inc.) 30 m \times 0.25 mm I.D. fused silica
Column temp.	40 $^{\circ}\text{C}$ (3 min) \rightarrow 140 $^{\circ}\text{C}$ (0 min)
Temp. rate	15 $^{\circ}\text{C}/\text{min}$
Injection temp.	200 $^{\circ}\text{C}$
Carrier gas	Helium
Column flow rate	1.0 mL/min
Hydrogen	40 mL/min
Air	400 mL/min
Sample size	1 μL
Injection method	Split
Split ratio	5:1
Detector	
Temp.	200 $^{\circ}\text{C}$
Sensitivity	Range 2^0

(b) Preparation of standard solution

The standard solutions to determine the concentration of the test item and 13F-EtOH in the sample for GC analysis were prepared as follows.

① Test item

20.5 μL [$30.7 \text{ mg} = 20.5 \text{ } \mu\text{L} \times 1.496 \text{ g/cm}^3$ (density)] of the test sample was taken out by microsyringe and dissolved in ethyl acetate to obtain 1020 mg/L solution of the test item. 307 mg/L standard solution was then prepared from this solution by dilution with ethyl acetate.

② 13F-EtOH

15.0 μL [$25.2 \text{ mg} = 15.0 \text{ } \mu\text{L} \times 1.678 \text{ g/cm}^3$ (density)] of authentic sample of 13F-EtOH (supplied by the sponsor)^{*5} was taken out by microsyringe and dissolved in ethyl acetate to obtain 839 mg/L solution of the 13F-EtOH. 252 mg/L standard solution was then prepared from this solution by dilution with ethyl acetate.

*5 Purity 99.8%

Lot number 180804

13F-EtOH was treated as 100% in purity.

(c) Calibration curve

① Test item

Standard solutions of 76.7, 153 and 307 mg/L were prepared by the same method as described in (b)①. These solutions were analyzed according to the analytical conditions described in (a). A calibration curve was drawn based on the relation between the peak area on the chromatograms and the respective concentrations (see Fig. 2).

② 13F-EtOH

Standard solutions of 62.9, 126 and 252 mg/L were prepared by the same method as described in (b)②. These solutions were analyzed according to the analytical conditions described in (a). A calibration curve was drawn based on the relation between the peak area on the chromatograms and the respective concentrations (see Fig. 3).

(2) Determination of 13F-AcOH

The samples for LC-MS analysis were analyzed under the following conditions. 13F-AcOH was detected as the negative ions of $m/z = 376.9$ and 754.8 in the LC-MS analysis. Therefore, these two ions were selected as measurement ions. The concentration of 13F-AcOH in the sample for LC-MS analysis was calculated proportionally by comparing the peak area on the total ion chromatogram of the sample for LC-MS analysis with that on the total ion chromatogram of 2.00 mg/L standard solution (see Table-7 and Fig. 10).

The lowest detectable peak area of 13F-AcOH was regarded as 800 considering the noise level, which corresponded to 13F-AcOH concentration of 0.019 mg/L.

(a) Analytical conditions

Instrument	Liquid chromatograph-mass spectrometer
HPLC system	Waters Corporation type Alliance2690
Mass spectrometer	Waters Corporation type ZMD

LC conditions

Column	L-column ODS (15 cm × 2.1 mm I.D., Chemicals Evaluation and Research Institute)
Column temp.	40°C
Eluent	A (80%) : Acetonitrile / formic acid (500/0.25 v/v) B (20%) : Water ^{*6} / formic acid (500/0.25 v/v)
Flow rate	0.2 mL/min
Sample size	1 µL

*6 City water was treated with ultrapure water system.

Mass conditions

Ionization mode	Electrospray ionization (ESI)
Detection ion	Negative
Detection mode	Selected ion monitoring (SIM)
Measurement ion (m/z)	376.9 and 754.8 (see Fig. 13)
Ion source temp.	120°C
Desolvation temp.	350°C
Cone voltage	20 V

(b) Preparation of standard solution

The standard solution to determine the concentration of 13F-AcOH in the sample for LC-MS analysis was prepared as follows.

100 mg of authentic sample of 13F-AcOH (supplied by the sponsor)^{*7} was accurately weighed and dissolved in acetonitrile to obtain 1000 mg/L solution of 13F-AcOH. 2.00 mg/L standard solution was then prepared from this solution by dilution with acetonitrile.

*7 Purity 99.4%
Lot number S6X01
13F-AcOH was treated as 100% in purity.

(c) Calibration curve

Standard solutions of 0.500, 1.00 and 2.00 mg/L were prepared by the same method as described in (b). These solutions were analyzed according to the analytical conditions described in (a). A calibration curve was drawn based on the relation between the peak area on the total ion chromatograms and the respective concentrations (see Fig. 4).

4.5.3 Recovery test and blank test

Each two test solutions (water + test item), two test solutions (sludge + test item), two test solutions (water + 13F-EtOH) and two test solutions (sludge + 13F-EtOH), two test solutions (water + 13F-AcOH) and two test solutions (sludge + 13F-AcOH) for recovery tests were prepared according to the methods described in Section 4.2. The test solutions were pretreated in accordance with the method described in Section 4.5.1, then analyzed according to the procedures and analytical conditions described in Section 4.5.2.

Each test solution for blank tests was prepared according to the method described in Section 4.2. The test solutions for blank tests were analyzed in the same way as the recovery tests. As for the blank tests, no peak appeared around the peaks of the test item, 13F-EtOH and 13F-AcOH on the chromatograms.

Two individual recovery rates and their averages of the test item, 13F-EtOH and 13F-AcOH on the analytical procedure are shown below. The average recovery rates were used as correction factors, for the determination of the test item, 13F-EtOH and 13F-AcOH in the analytical samples.

(1) Test item (see Table-2 and Fig. 6)

30.7 mg of the test sample was added in the recovery test.

Recovery rate in the test solutions (water + test item)

94.8%, 94.5% average 94.7%

Recovery rate in the test solutions (sludge + test item)

94.0%, 95.0% average 94.5%

(2) 13F-EtOH (see Table-3 and Fig. 7)

25.2 mg of authentic sample of 13F-EtOH was added in the recovery test.

Recovery rate in the test solutions (water + 13F-EtOH)

96.2%, 96.1% average 96.2%

Recovery rate in the test solutions (sludge + 13F-EtOH)

96.5%, 97.5% average 97.0%

(3) 13F-AcOH (see Table-4 and Fig. 8)

30 mg of authentic sample of 13F-AcOH was added in the recovery test.

Recovery rate in the test solutions (water + 13F-AcOH)

96.0%, 96.7% average 96.4%

Recovery rate in the test solutions (sludge + 13F-AcOH)

96.7%, 96.4% average 96.6%

4.6 Preparation and analysis of test solutions for determination of methacrylic acid

Besides the test solutions described in Section 4.2, the test solution (water + test item) and the test solution (sludge + test item) were prepared according to Section 4.2 and were cultivated for determination of methacrylic acid which was expected to be produced. During the cultivation, the appearance of the test solution was observed according to Section 4.4(1). After the end of the cultivation, methacrylic acid in the test solutions was determined.


(1) Conditions of cultivation

Cultivation method	Test vessel was the improved type for volatile substance whose volume was 300 mL. Each test solution was cultivated under the closed system performed by connecting the test vessel with air tank via tube. Absorbent for carbon dioxide described in Section 4.3(1) was attached to each test vessel.
Cultivation temperature	Approximately 25°C
Cultivation duration	28 days (under conditions of darkness) ^{*8}
Stirring method	Each test solution was stirred by a magnetic stirrer.
Room	Environmentally controlled room

^{*8} Cultivated from the experimental starting date to the experimental completion date described in page 2.

(2) Pretreatment of test solutions for analysis

The test solutions for the determination of methacrylic acid were pretreated to prepare samples for high-performance liquid chromatography (HPLC) analysis of methacrylic acid as follows.

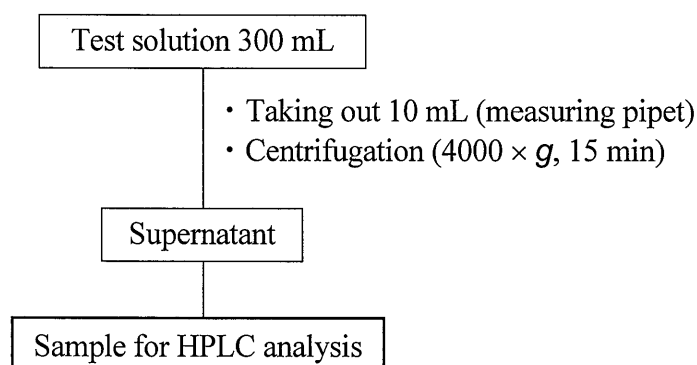

(3) Determination of methacrylic acid

The samples for HPLC analysis were analyzed under the following conditions. The concentration of methacrylic acid in the sample for HPLC analysis was calculated proportionally by comparing the peak area on the chromatogram of the sample for HPLC analysis with that on the chromatogram of 20.0 mg/L standard solution (see Table-8 and Fig. 11).

The lowest detectable peak area of methacrylic acid was regarded as 15000 $\mu\text{V} \cdot \text{sec}$ considering the noise level, which corresponded to methacrylic acid concentration of 0.20 mg/L.

(a) Analytical conditions

Instrument	High-performance liquid chromatograph
Pump	Shimadzu Corporation type LC-10AD _{VP}
Detector	Shimadzu Corporation type SPD-10AV _{VP}
Column oven	Shimadzu Corporation type CTO-10AC _{VP}
Auto injector	Shimadzu Corporation type SIL-10AD _{VP}
System controller	Shimadzu Corporation type SCL-10A _{VP}
Degasser	Shimadzu Corporation type DGU-14AM
Column	L-column ODS (15 cm \times 2.1 mm I.D., Chemicals Evaluation and Research Institute)
Column temp.	35°C
Eluent	A (30%) : Acetonitrile / phosphoric acid (1000/1 v/v) B (70%) : Water ^{*6} / phosphoric acid (1000/1 v/v)
Flow rate	0.2 mL/min
Measurement wavelength	205 nm (see Fig. 12)
Sample size	5 μL
Detector output	1 V/AU

(b) Preparation of standard solution

The standard solution to determine the concentration of methacrylic acid in the sample for HPLC analysis was prepared as follows.

100 mg of authentic sample of methacrylic acid (Wako Pure Chemical Industries, Ltd., reagent grade)^{*9} was accurately weighed and dissolved in purified water to obtain 1000 mg/L solution of methacrylic acid. 20.0 mg/L standard solution was then prepared from this solution by dilution with purified water.

^{*9} Methacrylic acid was treated as 100% in purity.

(c) Calibration curve

Standard solutions of 5.00, 10.0 and 20.0 mg/L were prepared by the same method as described in (b). These solutions were analyzed according to the analytical conditions described in (a). A calibration curve was drawn based on the relation between the peak area on the chromatograms and the respective concentrations (see Fig. 5).

4.7 Calculation of percentage biodegradation

The percentage biodegradations were calculated by the following equations and rounded off to the whole number.

(1) Percentage biodegradation by BOD

$$\text{Percentage biodegradation (\%)} = \frac{\text{BOD} - \text{B}}{\text{TOD}^{*10}} \times 100$$

BOD : Biochemical oxygen demand in the test solution
(sludge + test item) (experimental) (mg)

B : Biochemical oxygen demand in the control blank
(experimental) (mg)

TOD^{*10} : Theoretical oxygen demand required when the test
item was completely oxidized (theoretical) (mg)

*10 The purity was regarded as 100%.

(2) Percentage biodegradation of test item

$$\text{Percentage biodegradation (\%)} = \frac{\text{S}_w - \text{S}_s}{\text{S}_w} \times 100$$

S_s : Residual amount of the test item in the test solution
(sludge + test item) (experimental) (mg)

S_w : Residual amount of the test item in the test solution
(water + test item) (experimental) (mg)

4.7 Treatment of numerical values

Values were rounded off in accordance with JIS Z 8401:1999 rule B.

5. Validity of test conditions

The validity criteria of the test and the values in this test are shown in the following table.
This test was valid because all of the values in this test met the criteria.

		Value in present test	Value of criterion	See
Difference of extremes of replicate values of percentage biodegradation	Percentage biodegradation by BOD	5%	< 20%	Section 7.3 Percentage biodegradation
	Percentage Biodegradation of test item	11%		
Percentage biodegradation of aniline by BOD	After 7 days	62%	≥ 40%	Table-1 Fig.1
	After 14 days	72%	≥ 65%	
BOD value of control blank	After 28 days	7.7 mg	< 18 mg (< 60 mg/L)	Table-1 Fig. 1

6. Factors that affected reliability of test

No adverse effects on the reliability of this test were noted.

7. Results

7.1 Appearances of test solutions

Appearances of test media in cultivation vessels were as follows.

	Test solution	Appearance	pH
At the start of cultivation	Water + test item	The test item was not dissolved. The test solution was colorless.	-
	Sludge + test item	The test item was not dissolved. The test solution was colorless.	-
At the end of cultivation	Water + test item	Insoluble compound was observed. The test solution was colorless.	- ^{*11}
	Sludge + test item	Presence of insoluble compound except the sludge could not be judged. Growth of the sludge could not be judged. The test solution was colorless.	- ^{*11}

^{*11} After the end of the cultivation, the pH of the test solution (water + test item) and the test solutions (sludge + test item) was not measured because the test item was thought to be a volatile compound.

7.2 Analytical results of test solutions

Analytical results of the test solutions for the biodegradation test described in Section 4.2 after 28 days were as follows.

		Water + test item	Sludge + test item				Theoretical amount	Table	Fig.
		Vessel -1	Vessel -2	Vessel -3	Vessel -4				
BOD* ¹²	mg	0	4.8	3.4	4.2	30.1	1	1	
Residual amount and percentage residue of test item (GC)	mg	30.0	28.6	25.6	28.8	30.7	5	9	
	%①	98	93	83	94	-			
Produced amount and percentage production of 13F-EtOH (GC)	mg	0.6	2.6	4.2	1.3	25.9	6	9	
	%②	3	10	16	5	-			
Produced amount and percentage production of 13F-AcOH (LC-MS)	mg	0	0.6	0.6	1.4	26.9	7	10	
	%③	0	2	2	5	-			
Confirmation of production of methacrylic acid	-	Considering the loss of the test item and 13F-EtOH due to their volatilization in the pretreatment for analysis of methacrylic acid, methacrylic acid was not determined.					-	-	-
Mass balance of alkyl chain part (①+②+③)	%	101	105	101	104	-	-	-	

*12 The value of control blank was subtracted from the values of the test solutions (sludge + test item).

Analytical results of the additional test solutions for the determination of methacrylic acid described in Section 4.6 after 28 days were as follows.

		Water + test item	Sludge + test item	Theoretical amount	Table	Fig.
Produced amount and percentage production of methacrylic acid (HPLC)	mg	0	0	6.1	8	11
	%	0	0	-		

7.3 Percentage biodegradation

Percentage biodegradations of the test solution for the biodegradation test after 28 days were as follows.

		Sludge + test item				Table
		Vessel -2	Vessel -3	Vessel -4	Average	
Percentage biodegradation by BOD	%	16	11	14	14	1
Percentage biodegradation of test item (GC)	%	5	15	4	8	5

7.4 Discussion

(1) Analytical results


The percentage residue of the test item was as low as 98% and 83-94% in the test solution (water + test item) and the test solutions (sludge + test item), respectively. On the basis of these results, 2-(perfluorohexyl)ethanol (hereinafter referred to as 13F-EtOH), which was expected from results of the preliminary test prior to this study, in the test solutions was determined. As a result, 13F-EtOH was detected in the test solution (water + test item) and the test solutions (sludge + test item) (see Fig. 9). Mass balance of alkyl chain part of the test item calculated by sum of the percentage residue of the test item and the percentage production of 13F-EtOH (①+② in Section 7.2) was as high as 101% and 99-103% in the test solution (water + test item) and the test solutions (sludge + test item), respectively. Nevertheless, 3,3,4,4,5,5,6,6,7,7,8,8,8-tridecafluorooctanoic acid (hereinafter referred to as 13F-AcOH), which was also expected to be produced, in the test solutions was determined. As a result, the percentage production of 13F-AcOH was 2-5% in the test solutions (sludge + test item) (see Fig. 10). Mass balance of alkyl chain part of the test item recalculated by sum of the percentage residue of the test item and the percentage productions of 13F-EtOH and 13F-AcOH (①+②+③ in Section 7.2) was 100% in the test solutions (sludge + test item). Therefore, it was considered that the residues that had the alkyl chain part were the test item, 13F-EtOH and 13F-AcOH.

Considering the loss of the test item due to its volatilization in the pretreatment of the test solution for the determination of methacrylic acid [METI number (2)-1025, ready biodegradability], which was also expected to be produced, the additional test solutions were cultivated and were used for the determination of methacrylic acid in the test solutions. However, methacrylic acid was not detected in these test solutions (see Fig. 11). Then, methacrylic acid in the absorbents for carbon dioxide of the additional test solutions was determined because it was considered that methacrylic acid transferred from the test solution to the absorbent attached to the test vessel. As a result, methacrylic acid was detected in the absorbents, i.e. it was produced by hydrolysis of the test item (see Section 8.1).

As the result of the determination of methacrylic acid in the absorbents of the test solution (water + test item) for the biodegradation test, the percentage detection of methacrylic acid was 3% and was the same as the percentage production of 13F-EtOH (see Sections 7.2 and 8.1). Therefore, it was considered that all methacrylic acid transferred to the absorbent was recovered in the pretreatment described in Section 8.1. The percentage detection of methacrylic acid (1%, 2% and 1%, average 1%) was lower than sum of the percentage productions of 13F-EtOH and 13F-AcOH (12%, 18% and 10%, average 13%) in the test solutions (sludge + test item) for the biodegradation test (see Sections 7.2 and 8.1). These results suggested that some of the produced methacrylic acid was biodegraded in these test solutions. However, it was difficult to evaluate whether methacrylic acid was biodegraded from the percentage biodegradation by BOD, because the percentage biodegradation by BOD corresponding to difference between the percentage detection of methacrylic acid and the sum of the percentage productions of 13F-EtOH and 13F-AcOH (12%) was as low as 4%.

From the above discussions, it was considered that some of the test item was converted into methacrylic acid, 13F-EtOH and 13F-AcOH and that the rest of the test item, 13F-EtOH and 13F-AcOH remained in the test solution.


- *13 Percentage biodegradation by BOD when 12% of the theoretical amount of methacrylic acid was biodegraded.



Percentage biodegradation by BOD

$$= \{30.7 \times \text{C}_4\text{H}_6\text{O}_2 / \text{C}_{12}\text{H}_9\text{F}_{13}\text{O}_2 \times 12 / 100 \times 1.67\} / 30.1 \times 100 = 4(\%)$$

Conversion of test item in test solutions (sludge + test item) (presumption)

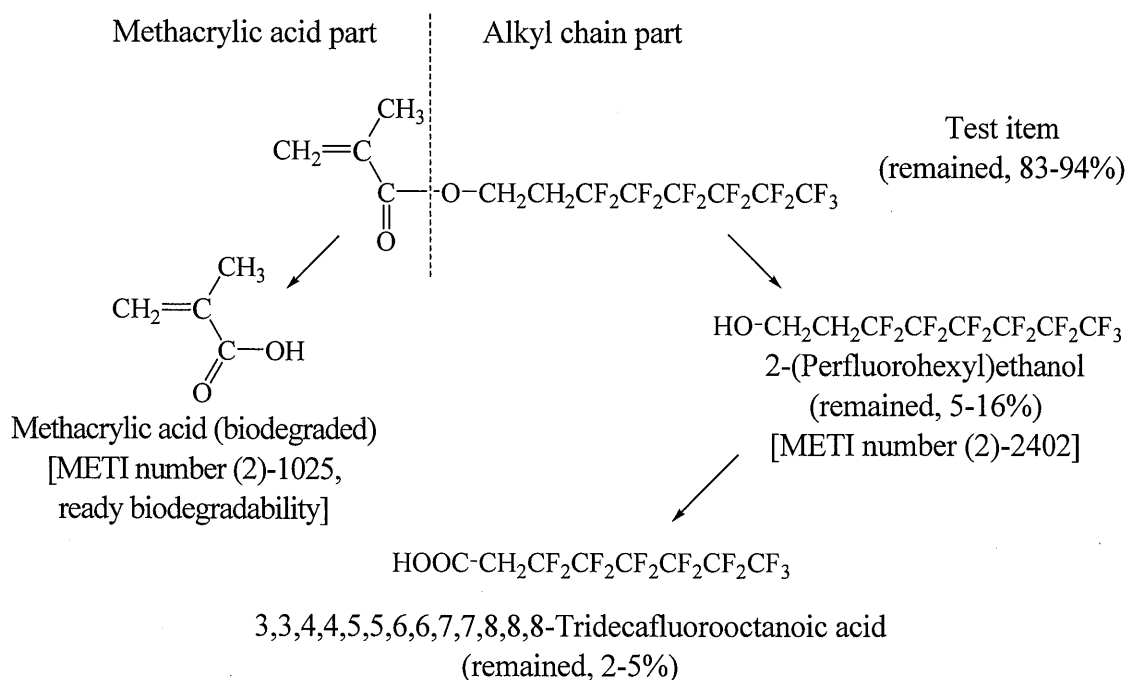

(2) Percentage biodegradation by BOD

As described in (1), the percentage biodegradation by BOD corresponding to the biodegraded amount of methacrylic acid was considered to be as low as 4%. Therefore, the main reason why the percentage biodegradation by BOD was 16%, 11% and 14% was considered to be the variation of the amount of background respiration of the activated sludge among the test solutions.

7.5 Conclusion


Some of the test item was converted into methacrylic acid, 2-(perfluorohexyl) ethanol and 3,3,4,4,5,5,6,6,7,7,8,8,8-tridecafluorooctanoic acid under the test conditions of this study. It was considered that some of methacrylic acid transferred from the test solution to the absorbent for carbon dioxide attached to the test vessel and that the other was biodegraded by microorganisms. The rest of the test item, 2-(perfluorohexyl) ethanol and 3,3,4,4,5,5,6,6,7,7,8,8,8-tridecafluorooctanoic acid remained in the test solution.

8. Remarks

8.1 Determination of methacrylic acid analysis in absorbents for carbon dioxide

Methacrylic acid was not detected in the additional test solutions in Section 4.6 and it was considered that the produced methacrylic acid transferred from the test solution to the absorbent for carbon dioxide attached to the test vessel. The absorbents of the test solutions for the determination of methacrylic acid were pretreated as follows and methacrylic acid was determined. Moreover, methacrylic acid in the absorbents of the test solutions for the biodegradation test was similarly determined because methacrylic acid was detected in the absorbents of the test solutions for the determination of methacrylic acid

(1) Pretreatment of the absorbents for carbon dioxide

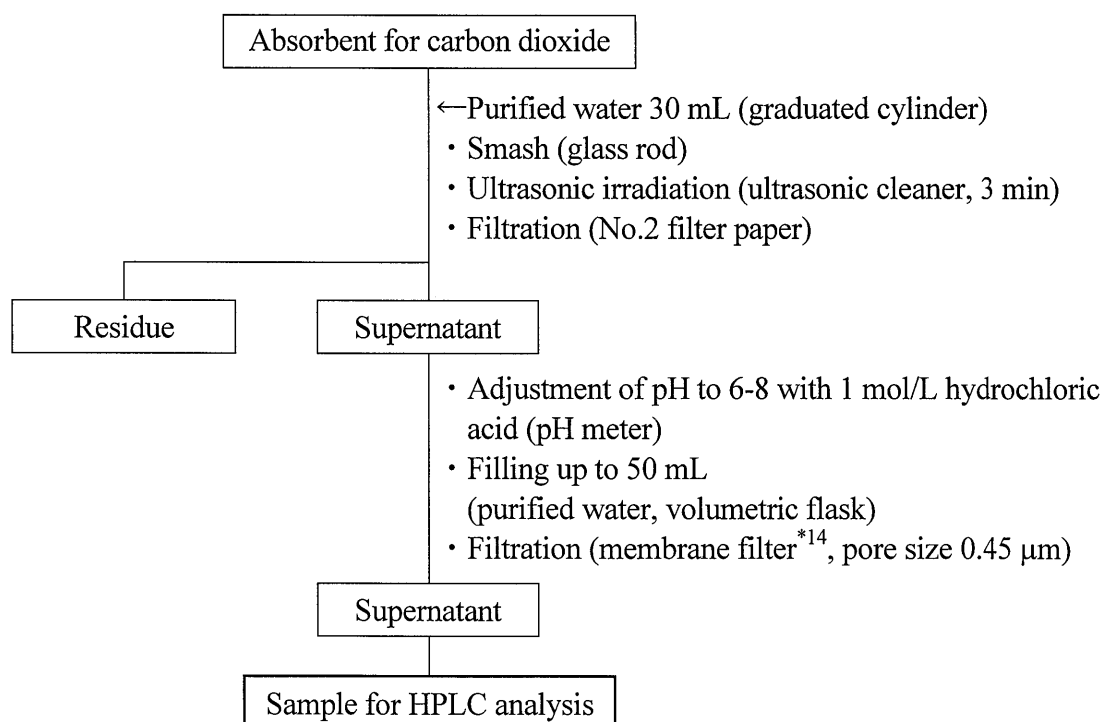

*14 Nuclepore Syrfil-MF

(2) Determination of methacrylic acid

See Section 4.6(3).

(3) Analytical results

Analytical results of the absorbents for carbon dioxide of the test solutions for the determination of methacrylic acid were as follows.

		Water + test item	Sludge + test item	Theoretical amount	Reference
Detected amount and percentage detection of methacrylic acid (HPLC)	mg	0.1	0.1	6.1	1, 4
	%	2	2	-	

Analytical results of the absorbents for carbon dioxide of the test solutions for the biodegradation test were as follows.

		Water + test item	Sludge + test item				Theoretical amount	Reference
		Vessel -1	Vessel -2	Vessel -3	Vessel -4			
Detected amount and percentage detection of methacrylic acid (HPLC)	mg	0.2	0.1	0.1	0.1	6.1	2, 5	
	%③	3	1	2	1	-		

8.2 Instruments used for test

Fourier transform infrared spectrophotometer :

Shimadzu Corporation type IRPrestige-21

Closed system oxygen consumption measuring apparatus :

see page 9

Gas chromatograph :

see page 11

Liquid chromatograph-mass spectrometer :

see page 13

High-performance liquid chromatograph :

see page 16

Electronic analytical balance :

Sartorius AG type BP210S

Ultraviolet and visible spectrophotometer :

JASCO Corporation type V-660

Refrigerated centrifuge :

KUBOTA Manufacturing Corporation
type 5922

Shaker :

Taitec Corporation type SR-2w

pH meter :

Toa Electronics Ltd. type HM-50G

Ultrasonic cleaner :

Yamato Scientific Co., Ltd type B-32H

8.3 Reagents used for analysis

Acetonitrile (HPLC grade) :	Wako Pure Chemical Industries, Ltd.
Purified water (Japanese Pharmacopeia) :	
	Takasugi Pharmaceutical Co., Ltd.
Ethyl acetate (reagent grade) :	Kanto Chemical Co., Inc.
Sodium chloride (reagent grade) :	MANAC Incorporated
Phosphoric acid (reagent grade) :	Wako Pure Chemical Industries, Ltd.
Formic acid (reagent grade) :	Wako Pure Chemical Industries, Ltd.
Methacrylic acid (reagent grade) :	Wako Pure Chemical Industries, Ltd.
1 mol/L Hydrochloric acid (for volumetric analysis) :	
	Wako Pure Chemical Industries, Ltd.
2-(Perfluorohexyl)ethanol :	Supplied by the sponsor
3,3,4,4,5,5,6,6,7,7,8,8,8-Tridecafluorooctanoic acid :	
	Supplied by the sponsor

Table-1 Calculation table for percentage biodegradation by BOD

Study No. 14739		Duration of cultivation: 28 days							
Vessel No.	7th day		14th day		21st day		28th day		Mean Deg. (%)
	BOD (mg)	Deg. (%)	BOD (mg)	Deg. (%)	BOD (mg)	Deg. (%)	BOD (mg)	Deg. (%)	
[5]	57.8	62	70.3	72	71.1	71	71.4	71	
[6]	1.7	-	5.3	-	7.1	-	7.7	-	
[2]	1.7	0	6.8	5	10.5	11	12.5	16	14
[3]	1.4	-1	5.9	2	9.2	7	11.1	11	
[4]	1.7	0	6.8	5	10.0	10	11.9	14	
[1]	0.0	-	0.0	-	0.0	-	0.0	-	

Deg. : Percentage biodegradation


Vessel No. [5] : Sludge + aniline
Vessel No. [6] : Control blank [B]
Vessel No. [2] [3] [4] : Sludge + test item
Vessel No. [1] : Water + test item

Test item of 30.7 mg was added.

Chart of BOD : Fig. 1

Deg. = $[\text{BOD} - \text{B}] / [\text{TOD}] \times 100 (\%)$


TOD of test item : 30.1 (mg)



$$13.25 \text{ O}_2 / \text{C}_{12}\text{H}_9\text{F}_{13}\text{O}_2 = 423.98 / 432.18 = 0.98$$

$$\text{TOD} = 30.7 \times 0.98 = 30.1 \text{ (mg)}$$

TOD of aniline : 90.3 (mg)



$$8.75 \text{ O}_2 / \text{C}_6\text{H}_7\text{N} = 279.99 / 93.13 = 3.01$$

$$\text{TOD} = 30 \times 3.01 = 90.3 \text{ (mg)}$$

Jan.10,2007 Name _____

Table-2 Calculation table for recovery rate of test item

Study No. 14739

Sample description	A	D	E	F
Standard solution 307mg/L	174335			
Water + test item -1	165284	29.1	94.8	94.7
Water + test item -2	164751	29.0	94.5	
Sludge + test item -1	163925	28.9	94.0	94.5
Sludge + test item -2	165554	29.2	95.0	
Control blank	n.d.			

Amount of test item added : 30.7 (mg)

A : Peak area ($\mu\text{V}\cdot\text{sec}$)

B : Final volume : 100 (mL)

C : Ratio of portion used for analysis : 300/300

D : Recovery amount (mg)

$$D_w = G \times (A(\text{Water} + \text{test item}) / A(\text{Standard})) \times (B / C) / 1000$$

$$D_s = G \times \{ (A(\text{Sludge} + \text{test item}) - A(\text{Control blank})) / A(\text{Standard}) \} \times (B / C) / 1000$$

E : Recovery rate (%)

$$E = D / 30.7 (\text{mg}) \times 100$$

F : Average recovery rate (%)

G : Concentration of standard solution : 307 (mg/L)

See Fig. 6

January 18, 2007

Name _____

Table-3 Calculation table for recovery rate of 13F-EtOH

Study No. 14739

Sample description	A	D	E	F
Standard solution 252mg/L	102048			
Water + 13F-EtOH -1	98210	24.3	96.2	96.2
Water + 13F-EtOH -2	98099	24.2	96.1	
Sludge + 13F-EtOH -1	98467	24.3	96.5	97.0
Sludge + 13F-EtOH -2	99470	24.6	97.5	
Control blank	n.d.			

Amount of 13F-EtOH added : 25.2 (mg)

A : Peak area ($\mu\text{V}\cdot\text{sec}$)

B : Final volume : 100 (mL)

C : Ratio of portion used for analysis : 300/300

D : Recovery amount (mg)

$$D_w = G \times (A(\text{Water} + 13\text{F-EtOH}) / A(\text{Standard})) \times (B / C) / 1000$$

$$D_s = G \times \{ (A(\text{Sludge} + 13\text{F-EtOH}) - A(\text{Control blank})) / A(\text{Standard}) \} \times (B / C) / 1000$$

E : Recovery rate (%)

$$E = D / 25.2 \text{ (mg)} \times 100$$

F : Average recovery rate (%)

G : Concentration of standard solution : 252 (mg/L)

See Fig. 7

January 18, 2007

Name _____

Table-4 Calculation table for recovery rate of 13F-AcOH

Study No. 14739

Sample description	A	D	E	F
Standard solution 2.00mg/L	91022			
Water + 13F-AcOH -1	87401	28.8	96.0	96.4
Water + 13F-AcOH -2	88009	29.0	96.7	
Sludge + 13F-AcOH -1	87989	29.0	96.7	96.6
Sludge + 13F-AcOH -2	87784	28.9	96.4	
Control blank	n.d.			

Amount of 13F-AcOH added : 30 (mg)

A : Peak area (-)

B : Final volume : 15 (mL)

C : Ratio of portion used for analysis : 1/10×1/100×300/300

D : Recovery amount (mg)

$$D_w = G \times (A(\text{Water} + 13\text{F-AcOH}) / A(\text{Standard})) \times (B / C) / 1000$$

$$D_s = G \times \{ (A(\text{Sludge} + 13\text{F-AcOH}) - A(\text{Control blank})) / A(\text{Standard}) \} \times (B / C) / 1000$$

E : Recovery rate (%)

$$E = D / 30 \text{ (mg)} \times 100$$

F : Average recovery rate (%)

G : Concentration of standard solution : 2.00 (mg/L)

See Fig. 8

January 18, 2007

Name _____

Table-5 Calculation table for percentage biodegradation of test item

Study No. 14739

Sample description	A	E	F	G	H
Standard solution 307mg/L	186406				
[1] Water + test item	172719	30.0	98		
[2] Sludge + test item	164291	28.6	93	5	
[3] Sludge + test item	147005	25.6	83	15	8
[4] Sludge + test item	165122	28.8	94	4	
[6] Control blank	n.d.				
<p>Amount of test item added : 30.7 (mg)</p> <p>A : Peak area ($\mu V \cdot sec$)</p> <p>B : Final volume : 100 (mL)</p> <p>C : Ratio of portion used for analysis : 300/300</p> <p>D : Recovery rate : 94.7 (%) (Water + test item) 94.5 (%) (Sludge + test item)</p> <p>E : Residual amount of test item (mg)</p> $E_w = I \times (A(\text{Water + test item}) / A(\text{Standard})) \times (B / C) / (D / 100) / 1000$ $E_s = I \times \{ (A(\text{Sludge + test item}) - A(\text{Control blank})) / A(\text{Standard}) \} \times (B / C) / (D / 100) / 1000$ <p>F : Percentage residue (%)</p> $F = E / 30.7 \text{ (mg)} \times 100$ <p>G : Percentage biodegradation (%)</p> $G = \{ (E(\text{Water + test item}) - E(\text{Sludge + test item})) / E(\text{Water + test item}) \} \times 100$ <p>H : Average percentage biodegradation (%)</p> <p>I : Concentration of standard solution : 307 (mg/L)</p> <p>See Fig. 9</p>					

January 31, 2007 Name

Table-6 Calculation table for percentage production of 13F-EtOH

Study No. 14739

Sample description	A	E	F	G
Standard solution 252mg/L	106133			
[1] Water + test item	2630	0.6	3	3
[2] Sludge + test item	10448	2.6	10	
[3] Sludge + test item	17160	4.2	16	10
[4] Sludge + test item	5355	1.3	5	
[6] Control blank	n.d.			
<p>Amount of test item added : 30.7 (mg)</p> <p>Theoretical amount of 13F-EtOH : 25.9 (mg)</p> $(30.7) \times (C_8H_5F_{13}O / C_{12}H_9F_{13}O_2)$ <p>A : Peak area ($\mu V \cdot sec$)</p> <p>B : Final volume : 100 (mL)</p> <p>C : Ratio of portion used for analysis : 300/300</p> <p>D : Recovery rate : 96.2 (%) (Water + test item)</p> <p>97.0 (%) (Sludge + test item)</p> <p>E : Amount of 13F-EtOH (mg)</p> $E_w = H \times (A(\text{Water + test item}) / A(\text{Standard})) \times (B / C) / (D / 100) / 1000$ $E_s = H \times \{ (A(\text{Sludge + test item}) - A(\text{Control blank})) / A(\text{Standard}) \}$ $\times (B / C) / (D / 100) / 1000$ <p>F : Percentage production (%)</p> $F = E / 25.9 \text{ (mg)} \times 100$ <p>G : Average percentage production (%)</p> <p>H : Concentration of standard solution : 252 (mg/L)</p> <p>See Fig. 9</p>				

January 22, 2007

Name _____

Table-7 Calculation table for percentage production of 13F-AcOH

Study No. 14739

Sample description	A	E	F	G
Standard solution 2.00mg/L	83124			
[1] Water + test item	n.d.	0	0	0
[2] Sludge + test item	1728	0.6	2	
[3] Sludge + test item	1714	0.6	2	3
[4] Sludge + test item	3715	1.4	5	
[6] Control blank	n.d.			

Amount of test item added : 30.7 (mg)
Theoretical amount of 13F-AcOH : 26.9 (mg)
 $(30.7) \times (C_8H_3F_{13}O_2 / C_{12}H_9F_{13}O_2)$

A : Peak area (-)
B : Final volume : 15 (mL)
C : Ratio of portion used for analysis : $1/10 \times 1/100 \times 300/300$
D : Recovery rate : 96.4 (%) (Water + test item)
96.6 (%) (Sludge + test item)
E : Amount of 13F-AcOH (mg)
 $E_w = H \times (A(\text{Water + test item}) / A(\text{Standard})) \times (B / C) / (D / 100) / 1000$
 $E_s = H \times \{ (A(\text{Sludge + test item}) - A(\text{Control blank})) / A(\text{Standard}) \}$
 $\times (B / C) / (D / 100) / 1000$
F : Percentage production (%)
 $F = E / 26.9 \text{ (mg)} \times 100$
G : Average percentage production (%)
H : Concentration of standard solution : 2.00 (mg/L)
See Fig. 10

January 22, 2007

Name _____

Table-8 Calculation table for percentage production of methacrylic acid
(test solution for analysis of methacrylic acid)

Study No. 14739

Sample description	A	D	E
Standard solution 20.0mg/L	1521555		
Water + test item	n.d.	0	0
Sludge + test item	n.d.	0	0
Control blank	n.d.		

Amount of test item added : 30.7 (mg)
Theoretical amount of methacrylic acid : 6.1 (mg)
 $(30.7) \times (C_4H_6O_2 / C_{12}H_9F_{13}O_2)$

A : Peak area ($\mu V \cdot sec$)
B : Final volume : 10 (mL)
C : Ratio of portion used for analysis : 10/300
D : Amount of methacrylic acid (mg)
 $D_w = F \times (A(\text{Water + test item}) / A(\text{Standard})) \times (B / C) / 1000$
 $D_s = F \times \{ (A(\text{Sludge + test item}) - A(\text{Control blank})) / A(\text{Standard}) \} \times (B / C) / 1000$
E : Percentage production (%)
 $E = D / 6.1 \text{ (mg)} \times 100$
F : Concentration of standard solution : 20.0 (mg/L)

See Fig. 11

January 31, 2007

Name _____

Reference 1 Calculation table for percentage detection of methacrylic acid
(CO₂ absorbent, test solution for analysis of methacrylic acid)

Study No. 14739

Sample description	A	D	E
Standard solution 20.0mg/L	1518705		
Water + test item	225650	0.1	2
Sludge + test item	140937	0.1	2
Control blank	n.d.		

Amount of test item added : 30.7 (mg)
Theoretical amount of methacrylic acid : 6.1 (mg)
 $(30.7) \times (C_4H_6O_2 / C_{12}H_9F_{13}O_2)$

A : Peak area ($\mu V \cdot sec$)
B : Final volume : 50 (mL)
C : Ratio of portion used for analysis : 1
D : Amount of methacrylic acid (mg)
 $D_w = F \times (A(\text{Water} + \text{test item}) / A(\text{Standard})) \times (B / C) / 1000$
 $D_s = F \times \{ (A(\text{Sludge} + \text{test item}) - A(\text{Control blank})) / A(\text{Standard}) \} \times (B / C) / 1000$
E : Percentage detection (%)
 $E = D / 6.1 \text{ (mg)} \times 100$
F : Concentration of standard solution : 20.0 (mg/L)

See Reference 4

January 31, 2007

Name _____

Reference 2 Calculation table for percentage detection of methacrylic acid
(CO₂ absorbent)

Study No. 14739

Sample description	A	D	E	F
Standard solution 20.0mg/L	1523373			
[1] Water + test item	275549	0.2	3	3
[2] Sludge + test item	103843	0.1	1	
[3] Sludge + test item	165511	0.1	2	1
[4] Sludge + test item	108086	0.1	1	
[6] Control blank	n.d.			

Amount of test item added : 30.7 (mg)
Theoretical amount of methacrylic acid : 6.1 (mg)
 $(30.7) \times (C_4H_6O_2 / C_{12}H_9F_{13}O_2)$

A : Peak area ($\mu V \cdot sec$)
B : Final volume : 50 (mL)
C : Ratio of portion used for analysis : 1
D : Amount of methacrylic acid (mg)
 $D_w = G \times (A(\text{Water} + \text{test item}) / A(\text{Standard})) \times (B / C) / 1000$
 $D_s = G \times \{ (A(\text{Sludge} + \text{test item}) - A(\text{Control blank})) / A(\text{Standard}) \} \times (B / C) / 1000$
E : Percentage detection (%)
 $E = D / 6.1 \text{ (mg)} \times 100$
F : Average percentage detection (%)
G : Concentration of standard solution : 20.0 (mg/L)
See Reference 5

January 31, 2007

Name _____

Study No. 14739

(Test item 13F-SFMA)

Cultivating conditions:

Concentration

Test item 100 (mg/L)

Reference item (aniline) 100 (mg/L)

Activated sludge 30 (mg/L)

Temperature 25 ± 1 °C

Duration 28 days (Dec.13,2006 - Jan.10,2007)

Note: —

Vessel No.	Sample Description	BOD (mg)			
		7th day	14th day	21st day	28th day
[1]	Water + test item	0.0	0.0	0.0	0.0
[2]	Sludge + test item	1.7	6.8	10.5	12.5
[3]	Sludge + test item	1.4	5.9	9.2	11.1
[4]	Sludge + test item	1.7	6.8	10.0	11.9
[5]	Sludge + aniline	57.8	70.3	71.1	71.4
[6]	Control blank [B]	1.7	5.3	7.1	7.7

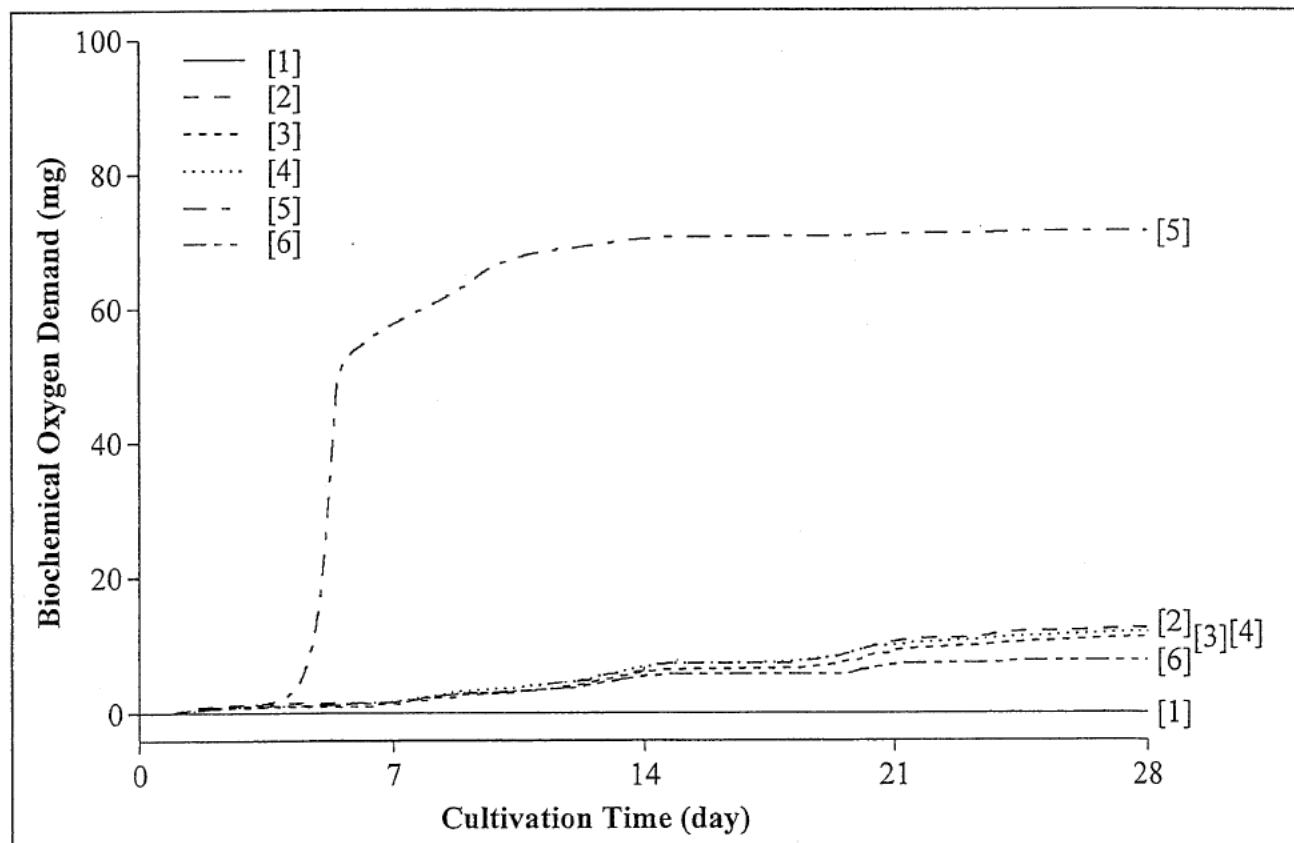


Fig. 1 Chart of BOD.

Jan.10,2007 Name _____


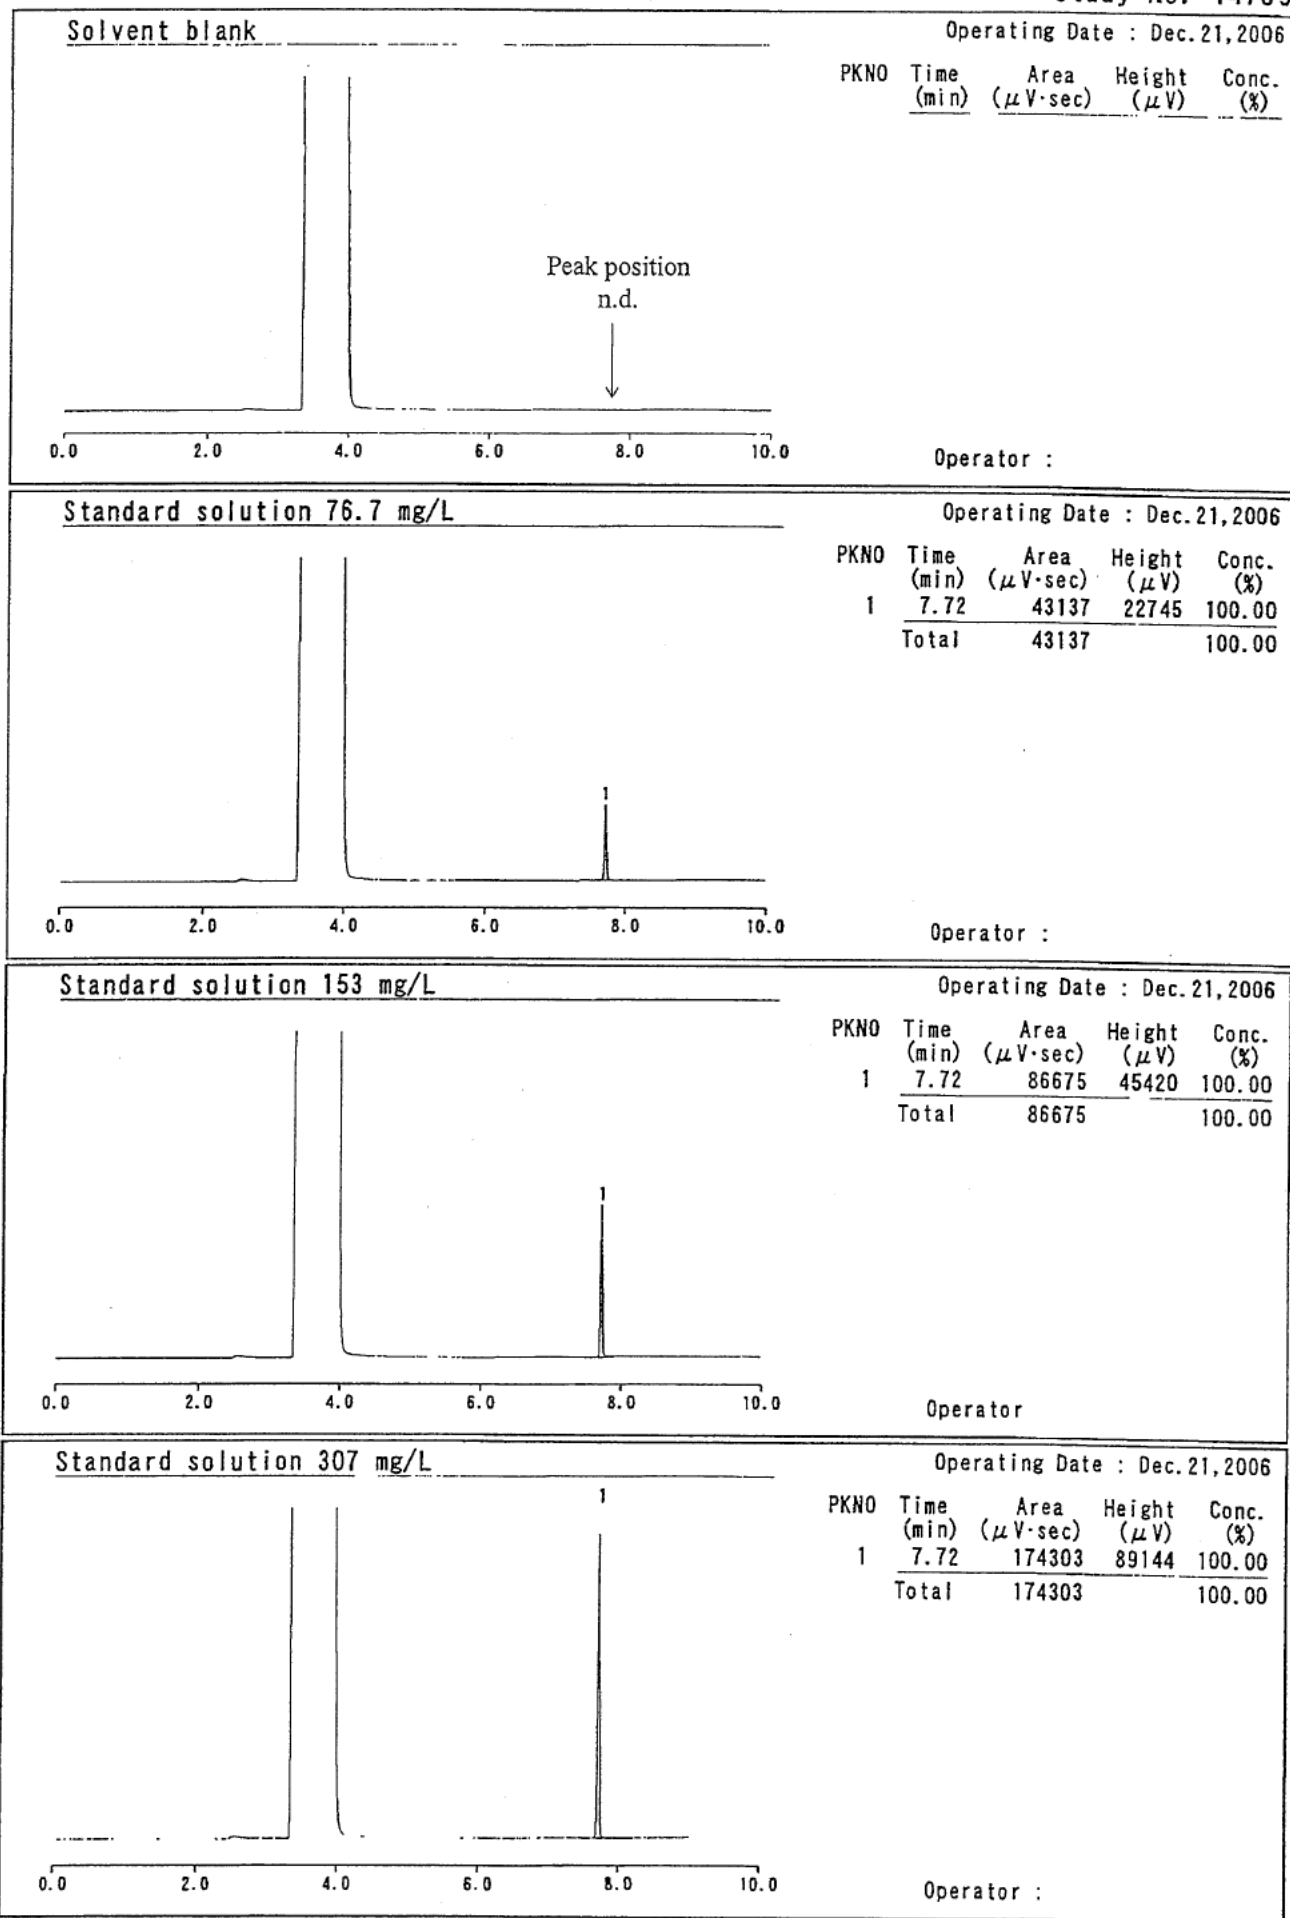


Fig. 2 - 1 Chromatograms of GC analysis for calibration curve (test item).

Date : Dec. 21, 2006 Name : _____

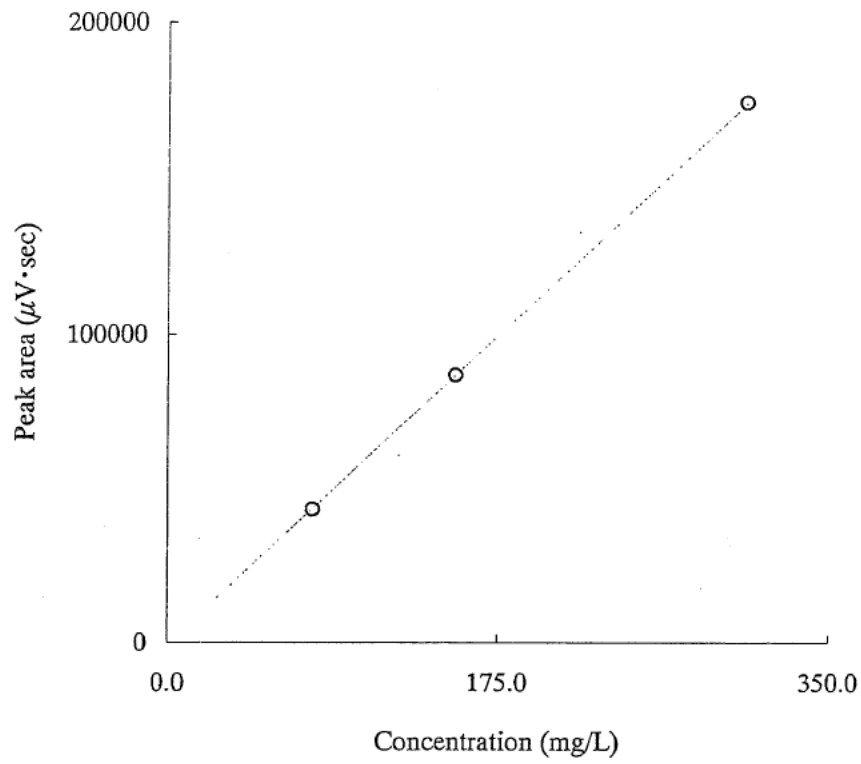

$$y = 567x$$

$$r = 1.00$$

Concentration (mg/L)	Peak area ($\mu\text{V}\cdot\text{sec}$)
76.7	43137
153	86675
307	174303

Fig. 2 - 2 Calibration curve of test item.

December 21, 2006

Name _____


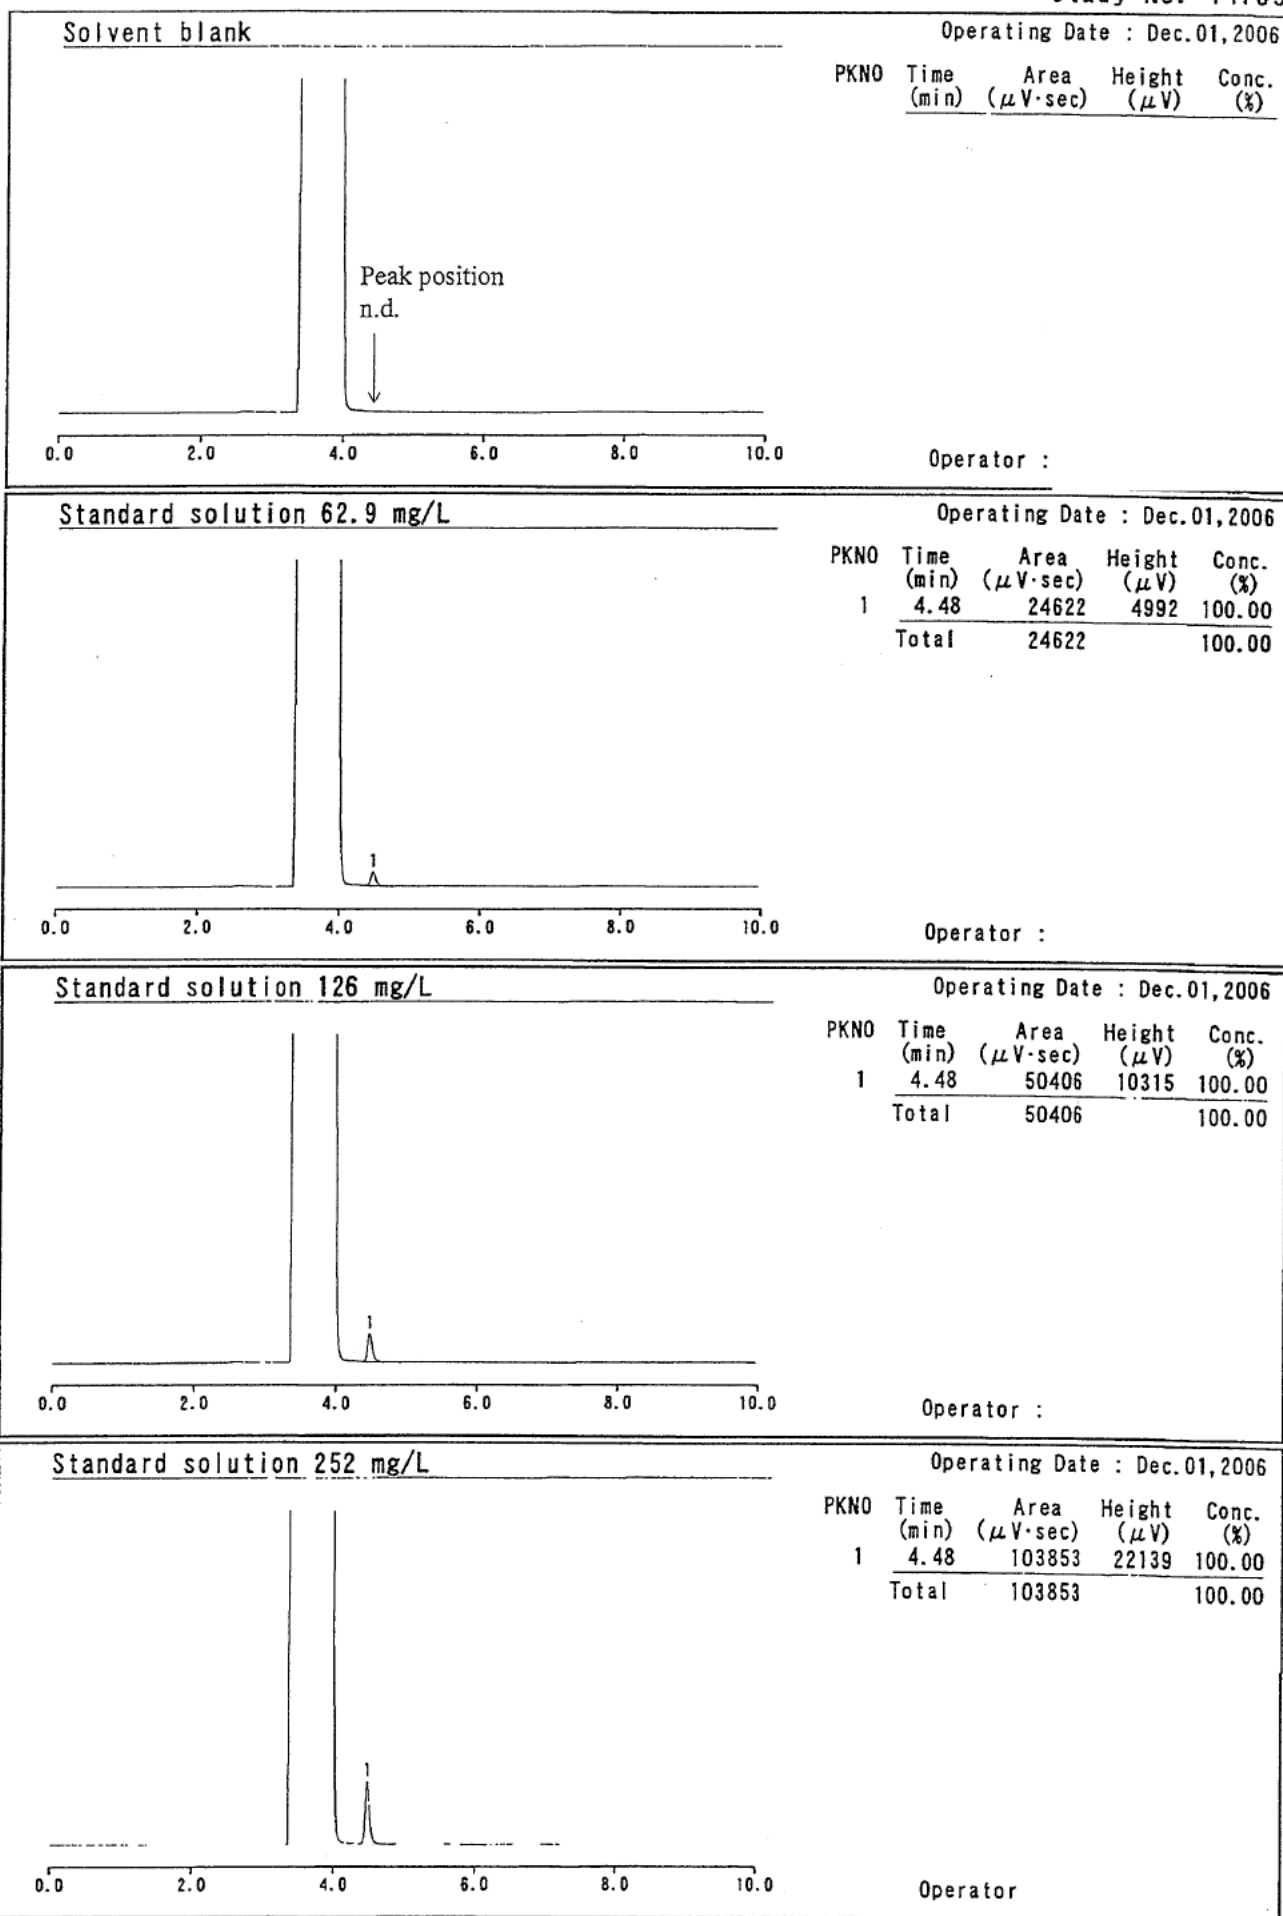


Fig 3 - 1

Chromatograms of GC analysis for calibration curve (13F-EtOH).

Date : Dec.1,2006 Name : _____

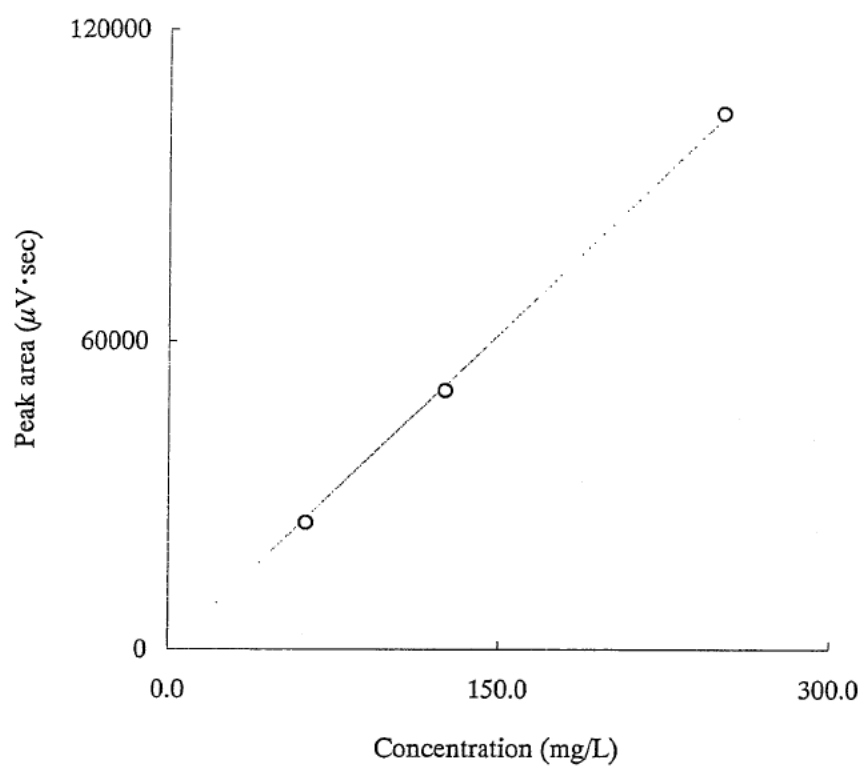

$$y = 409x$$

$$r = 1.00$$

Concentration (mg/L)	Peak area (μV·sec)
62.9	24622
126	50406
252	103853

Fig. 3 - 2 Calibration curve of 13F-EtOH.

December 1, 2006

Name _____


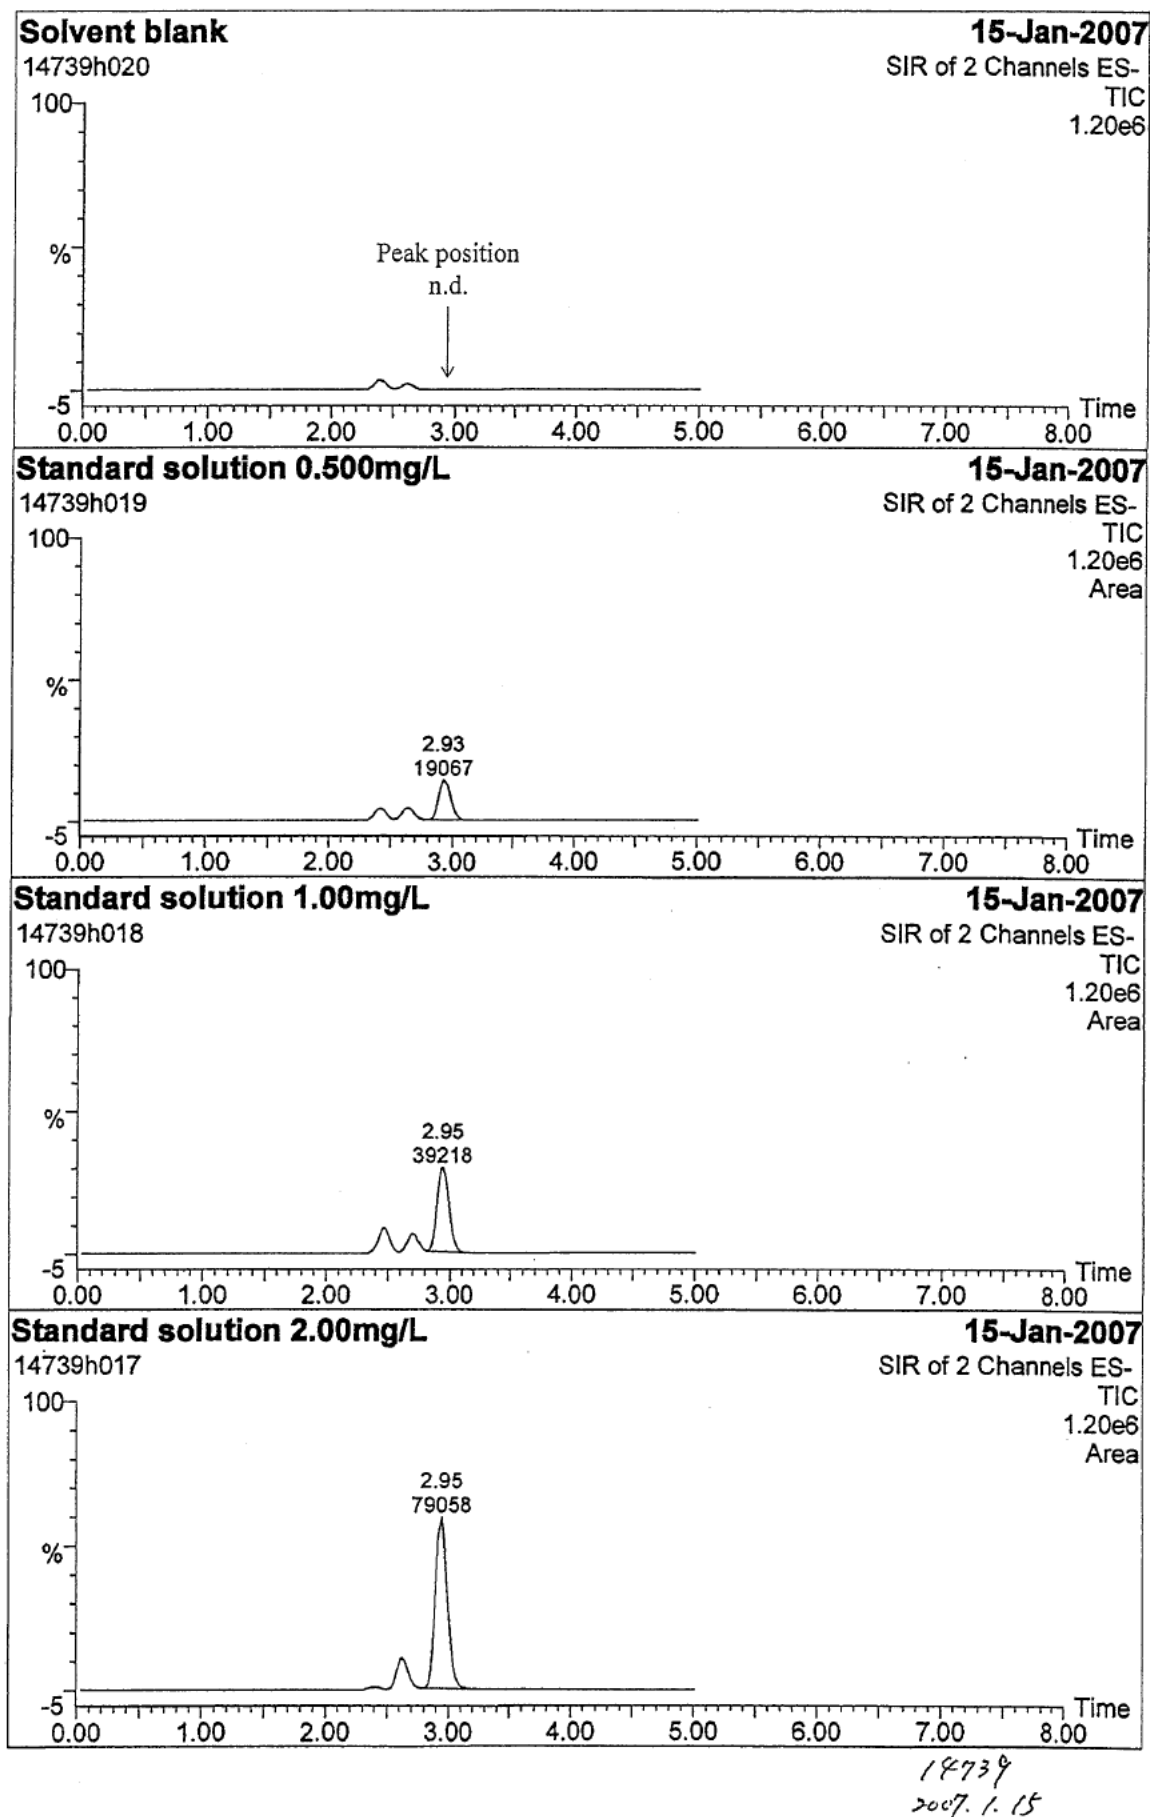


Fig. 4 - 1 Total ion chromatograms of LC-MS analysis for calibration curve (13F-AcOH).

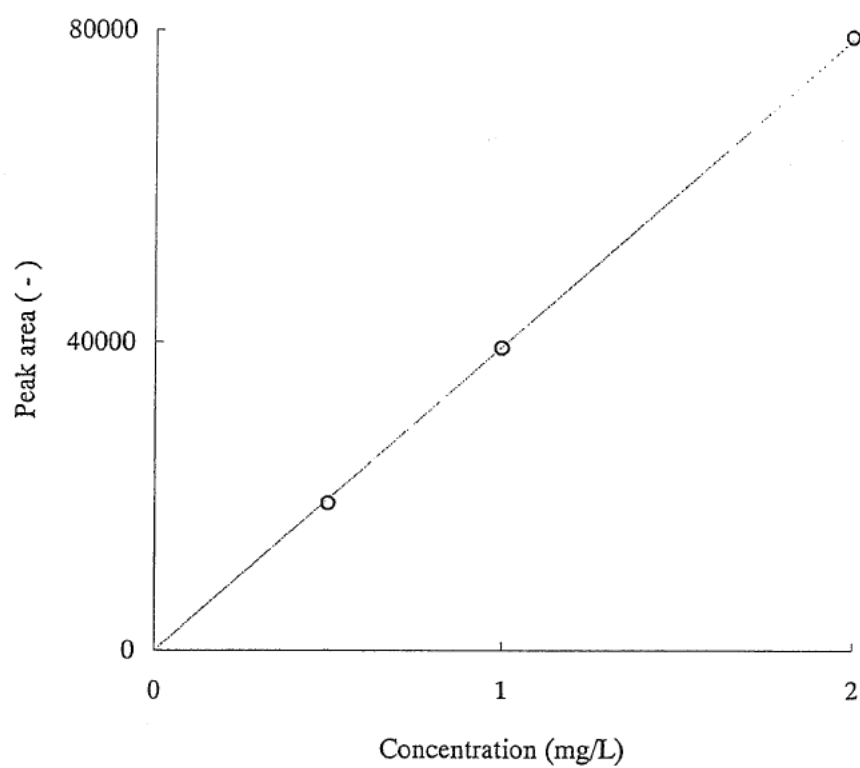

Concentration (mg/L)	Peak area (-)
0.500	19067
1.00	39218
2.00	79058

Fig. 4 - 2 Calibration curve of 13F-AcOH.


January 15, 2007

Name _____

Solvent blank

Operating Date : Jan. 10, 2007

PKNO	Time (min)	Area ($\mu\text{V}\cdot\text{sec}$)	Height (μV)	Conc. (%)
------	------------	---------------------------------------	--------------------------	-----------

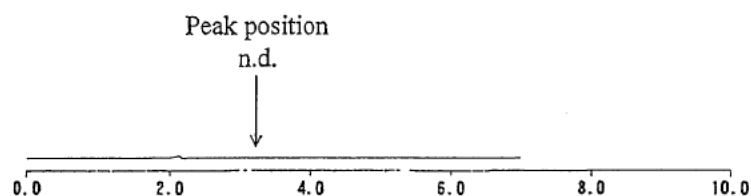


Operator :

Standard solution 5.00 mg/L

Operating Date : Jan. 10, 2007

PKNO	Time (min)	Area ($\mu\text{V}\cdot\text{sec}$)	Height (μV)	Conc. (%)
1	3.22	387145	79357	100.00
Total		387145		100.00

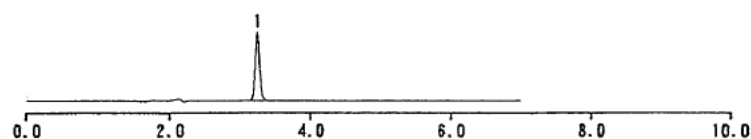


Operator :

Standard solution 10.0 mg/L

Operating Date : Jan. 10, 2007

PKNO	Time (min)	Area ($\mu\text{V}\cdot\text{sec}$)	Height (μV)	Conc. (%)
1	3.22	768474	157228	100.00
Total		768474		100.00

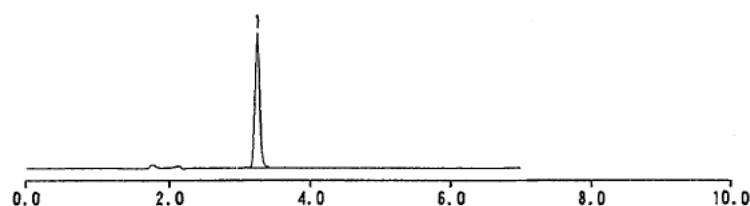


Operator :

Standard solution 20.0 mg/L

Operating Date : Jan. 10, 2007

PKNO	Time (min)	Area ($\mu\text{V}\cdot\text{sec}$)	Height (μV)	Conc. (%)
1	3.22	1527115	311809	100.00
Total		1527115		100.00

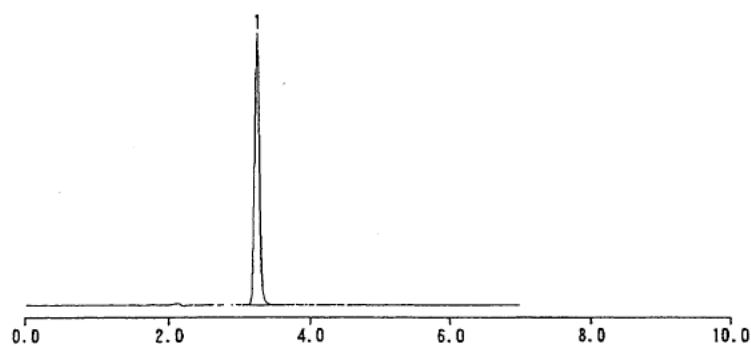


Operator :

Fig. 5 - 1

Chromatograms of HPLC analysis for calibration curve (methacrylic acid).

Date : Jan. 10, 2007 Name : _____

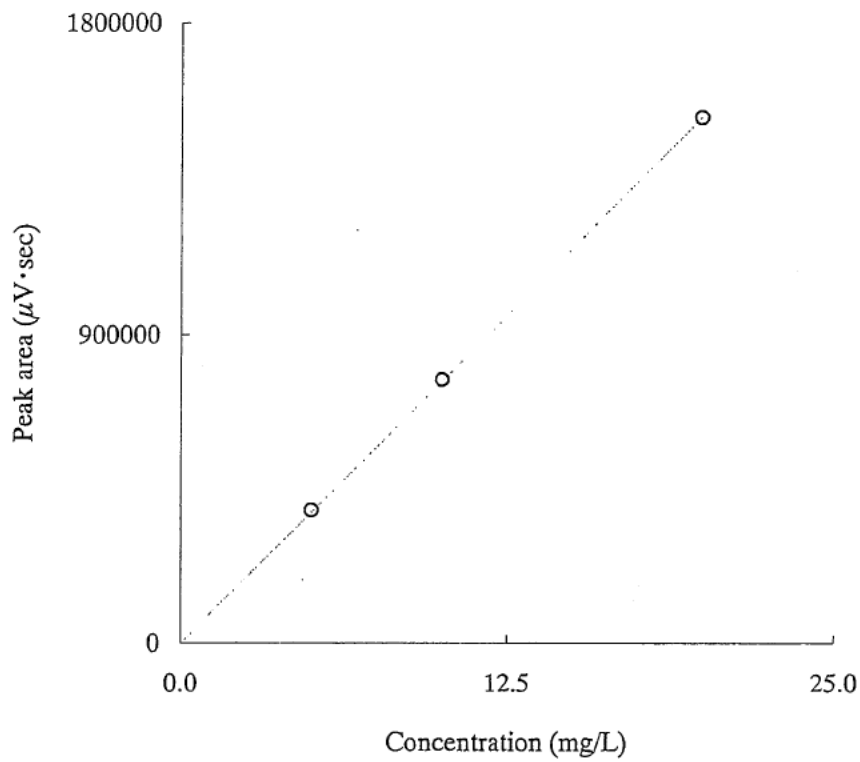

$$y = 76501x$$

$$r = 1.00$$

Concentration (mg/L)	Peak area (μV·sec)
5.00	387145
10.0	768474
20.0	1527115

Fig. 5 - 2 Calibration curve of methacrylic acid.

January 16, 2007

Name _____

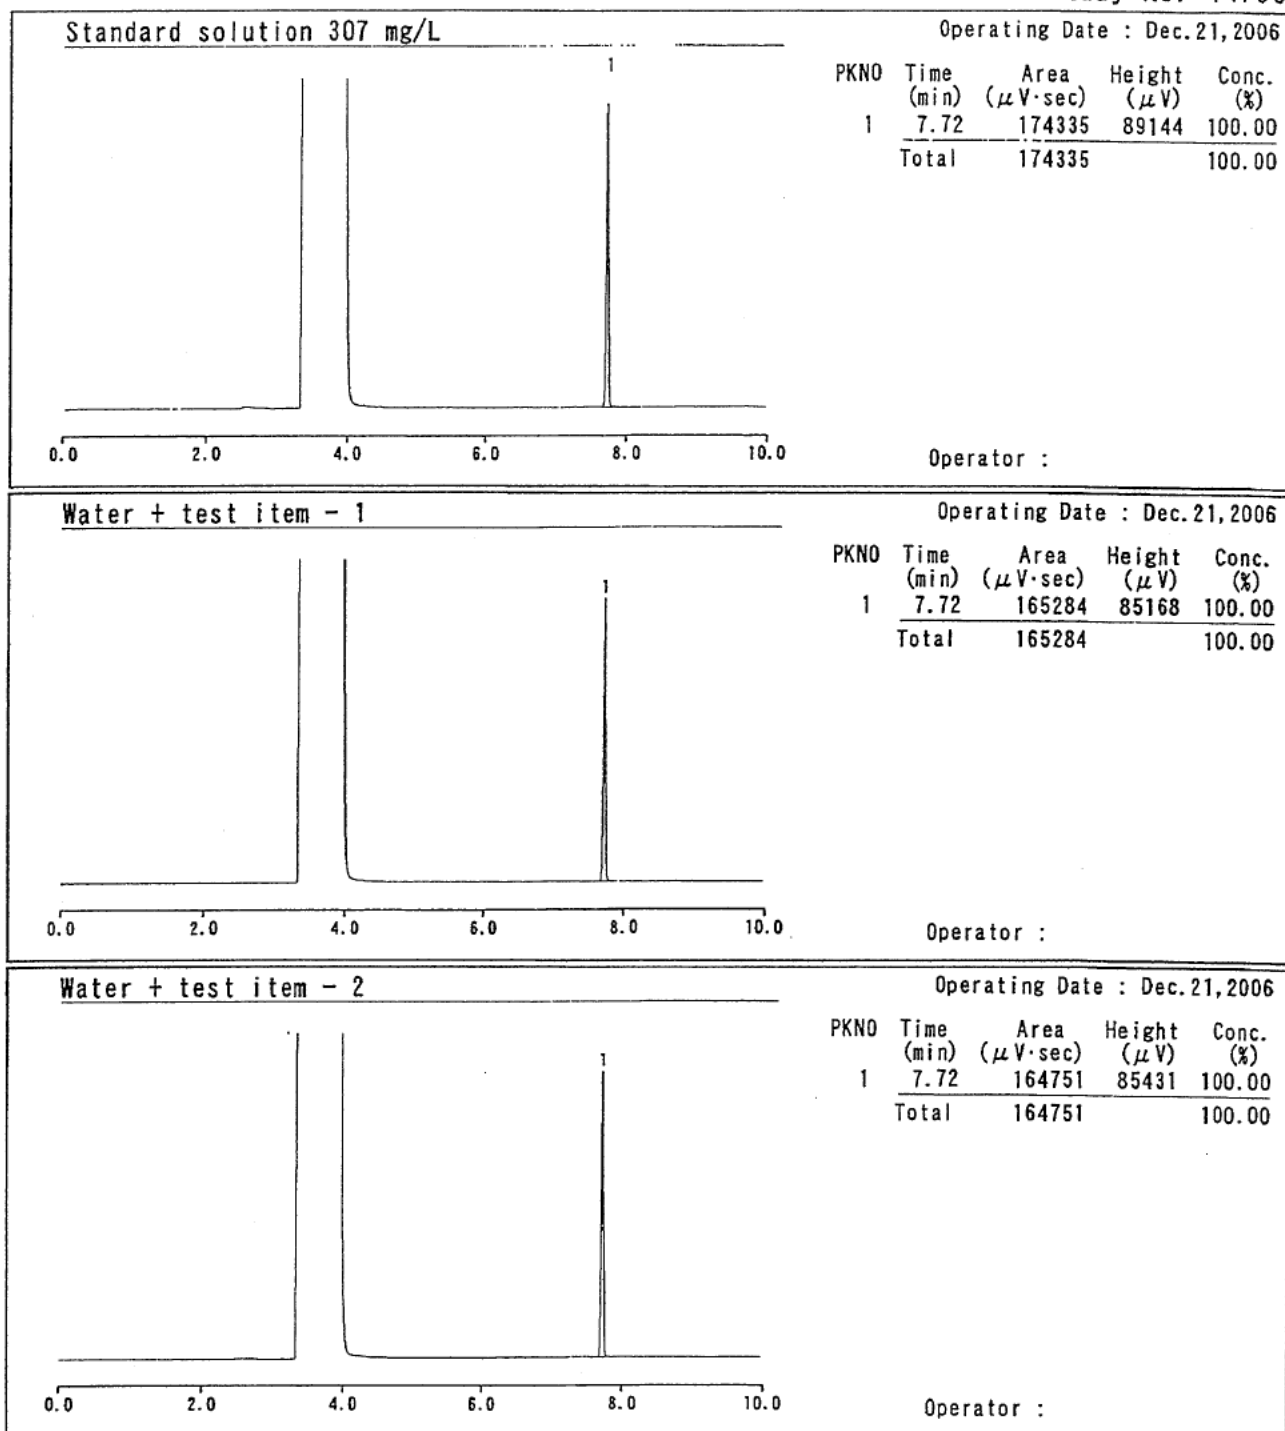


Fig.6 - 1 Chromatograms of GC analysis for recovery test (test item).

Date : Dec.21,2006 Name : _____

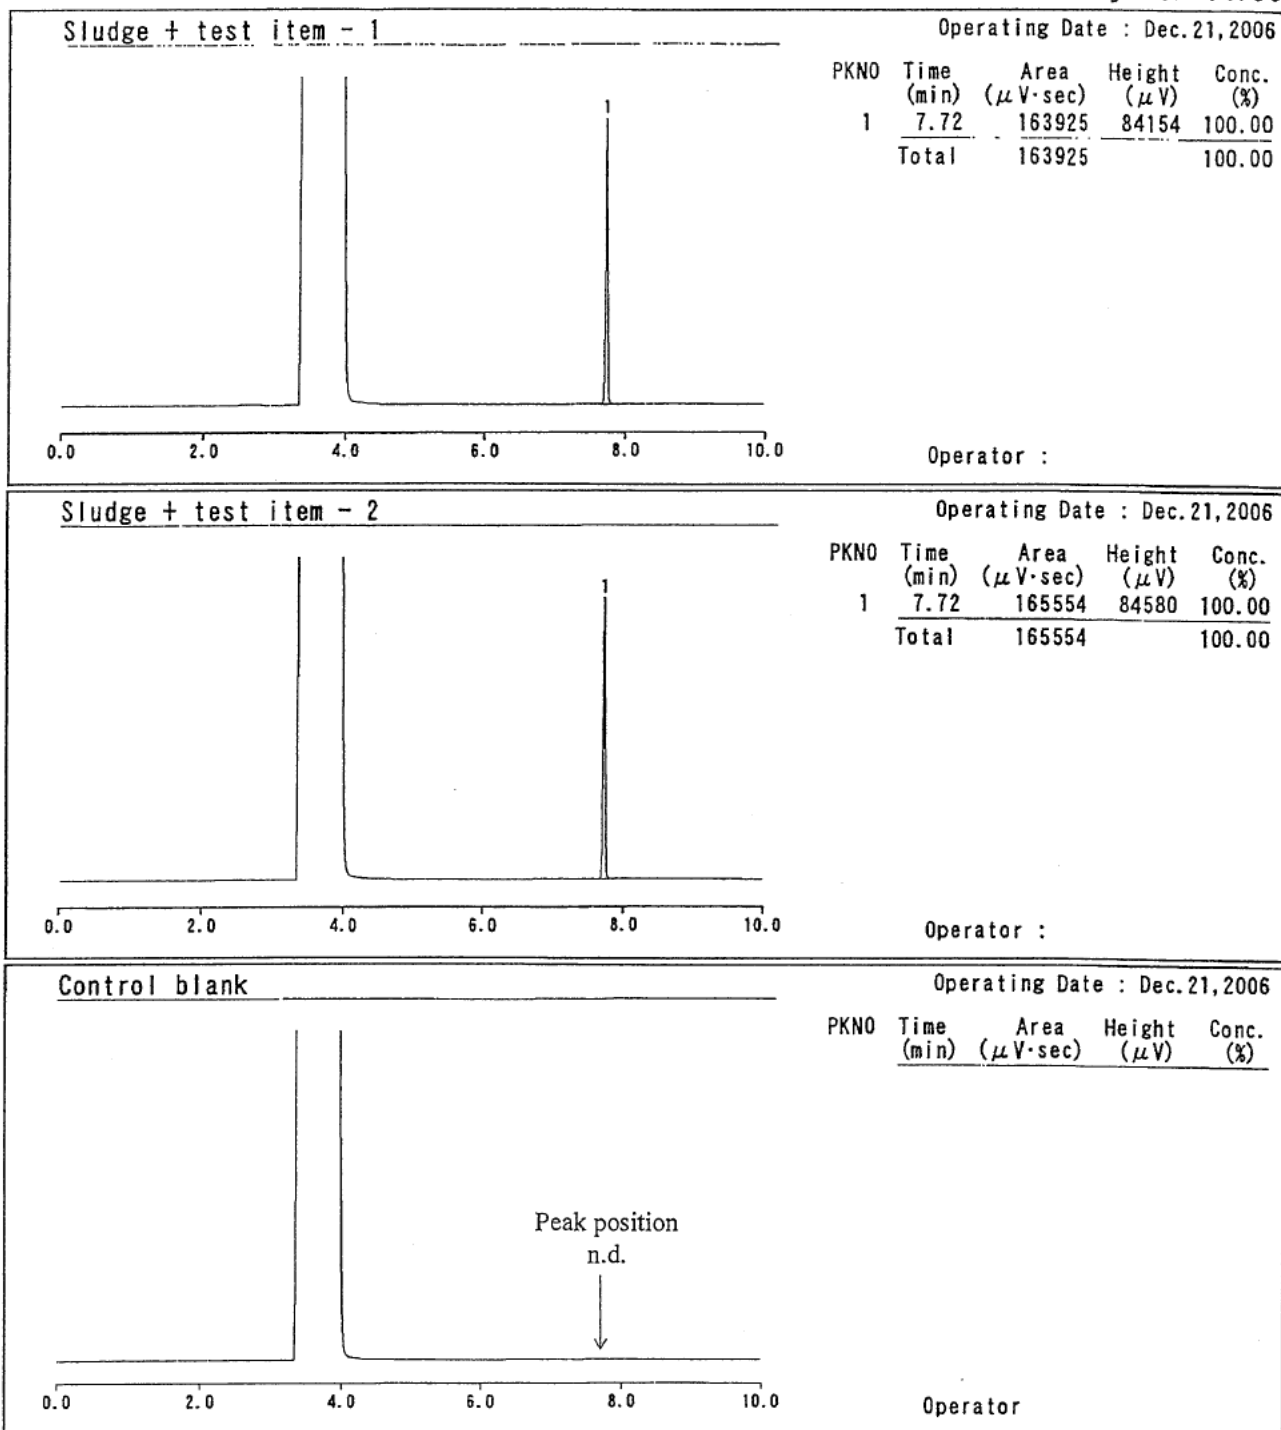


Fig.6 - 2

Chromatograms of GC analysis for recovery test (test item).

Date : Dec.21,2006 Name : _____

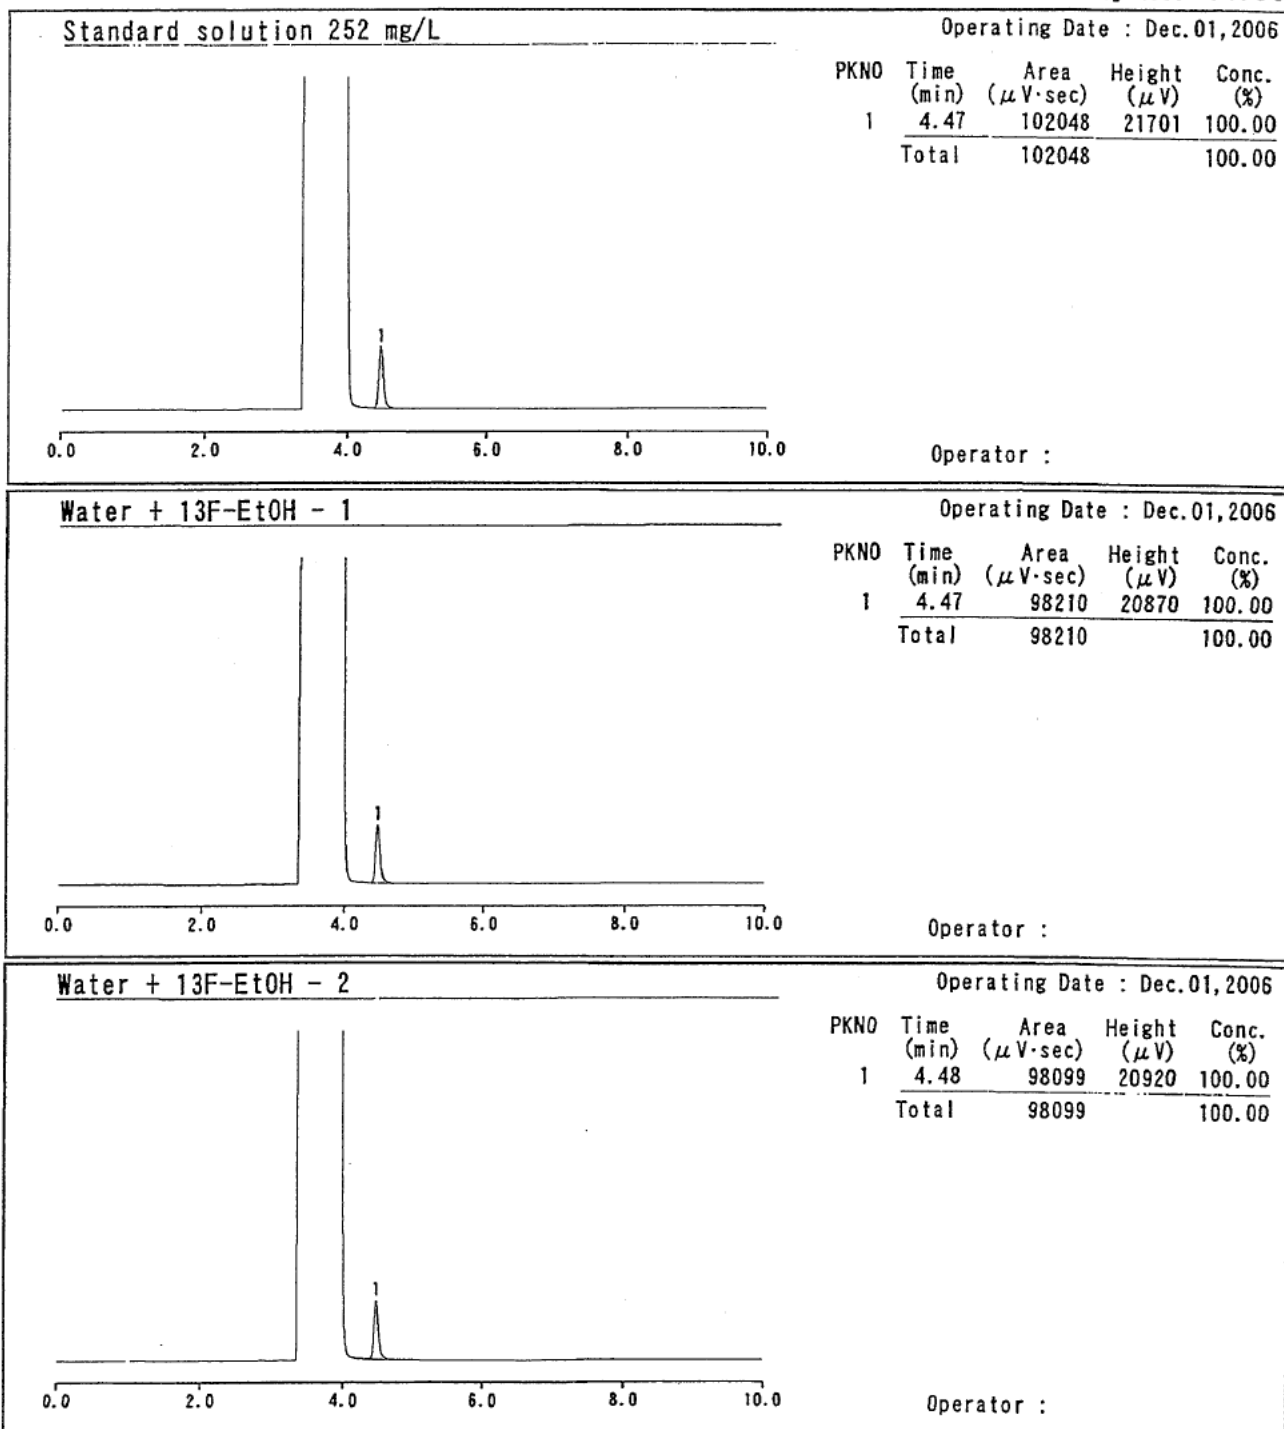


Fig.7 - 1 Chromatograms of GC analysis for recovery test (13F-EtOH).

Date : Dec.5,2006 Name : _____

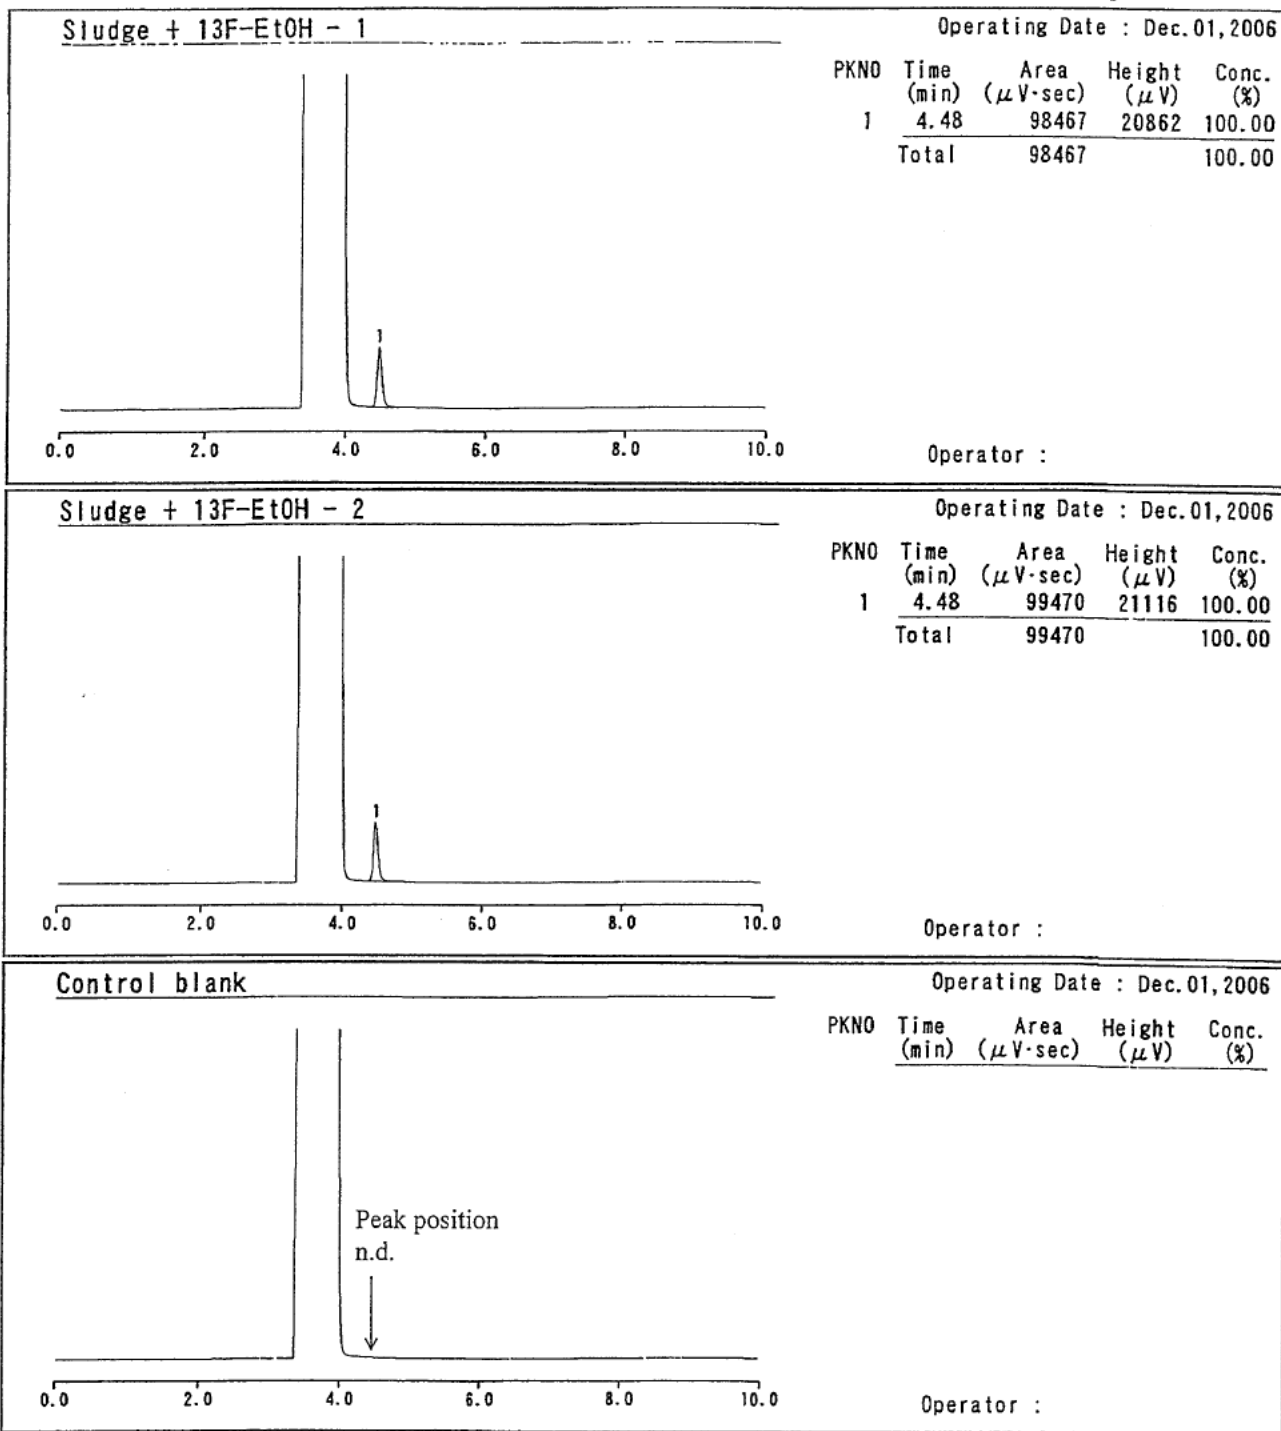


Fig.7 - 2 Chromatograms of GC analysis for recovery test (13F-EtOH).

Date : Dec.5,2006 Name : _____

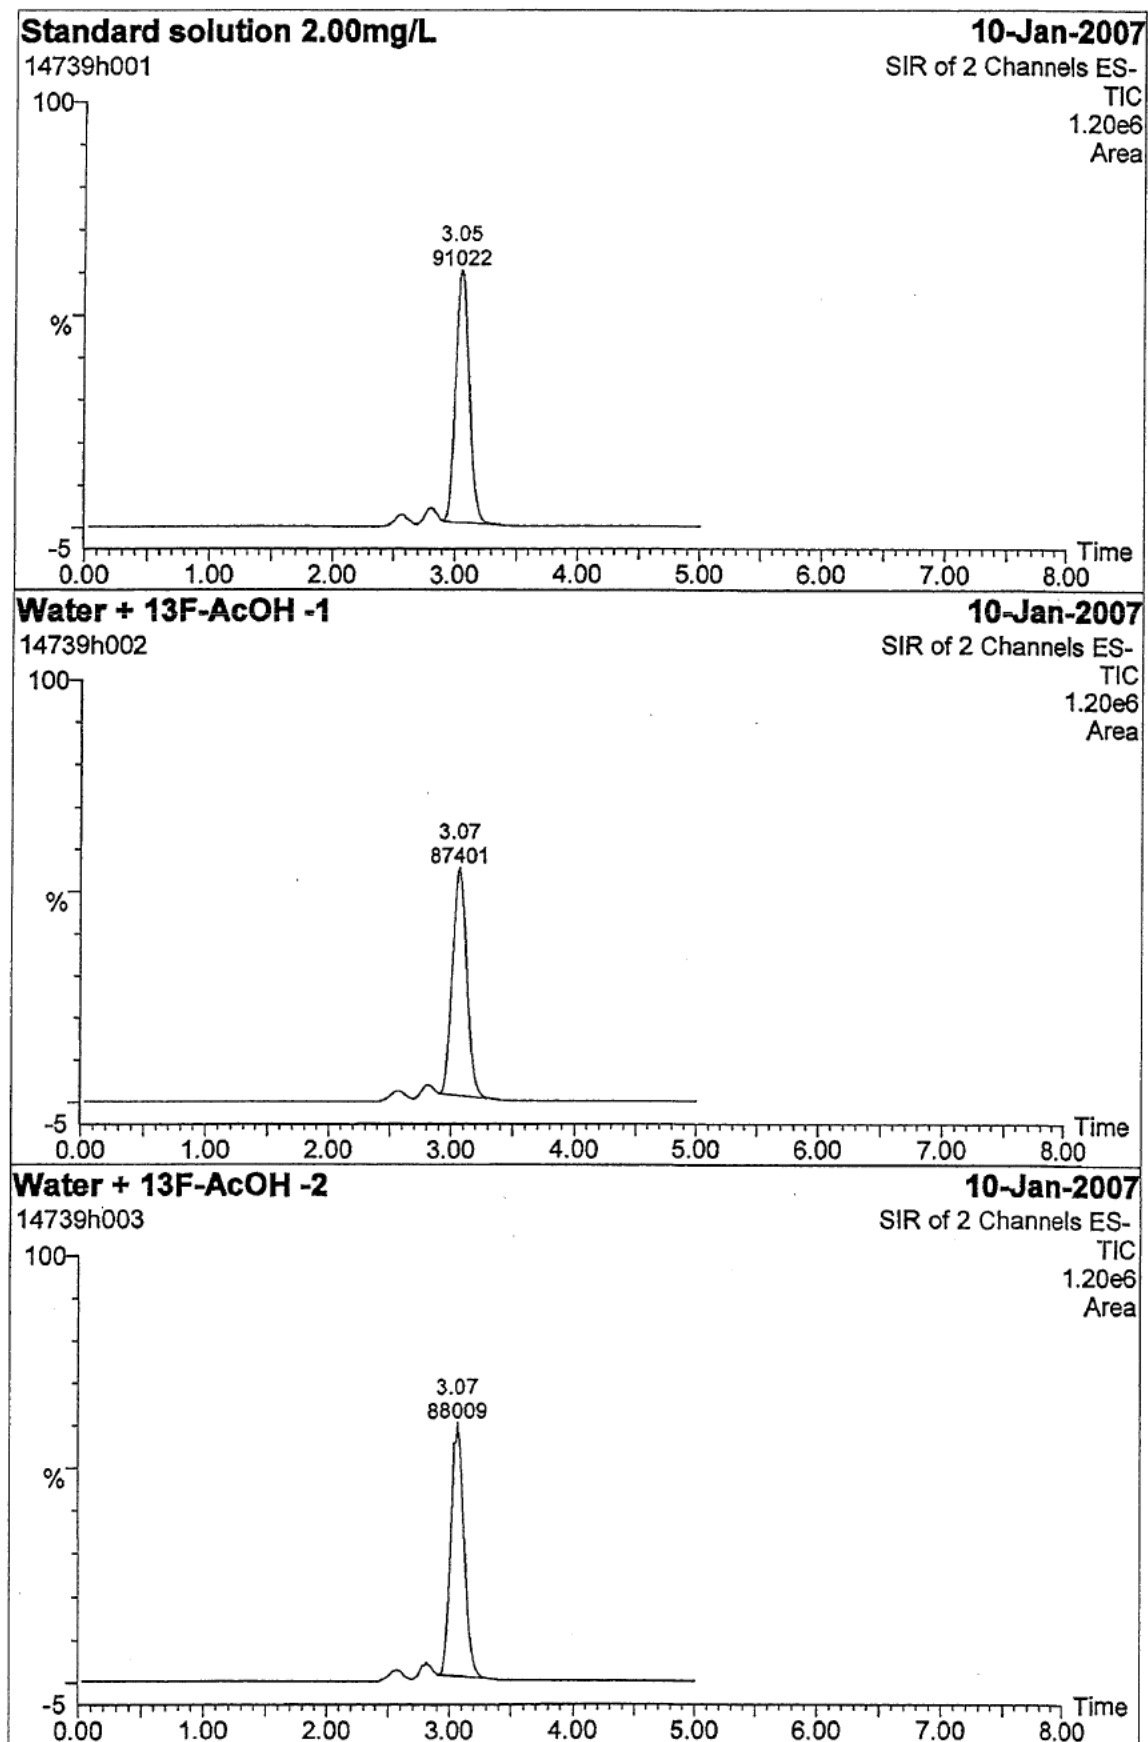


Fig. 8 - 1 Total ion chromatograms of LC-MS analysis for recovery test (13F-AcOH).

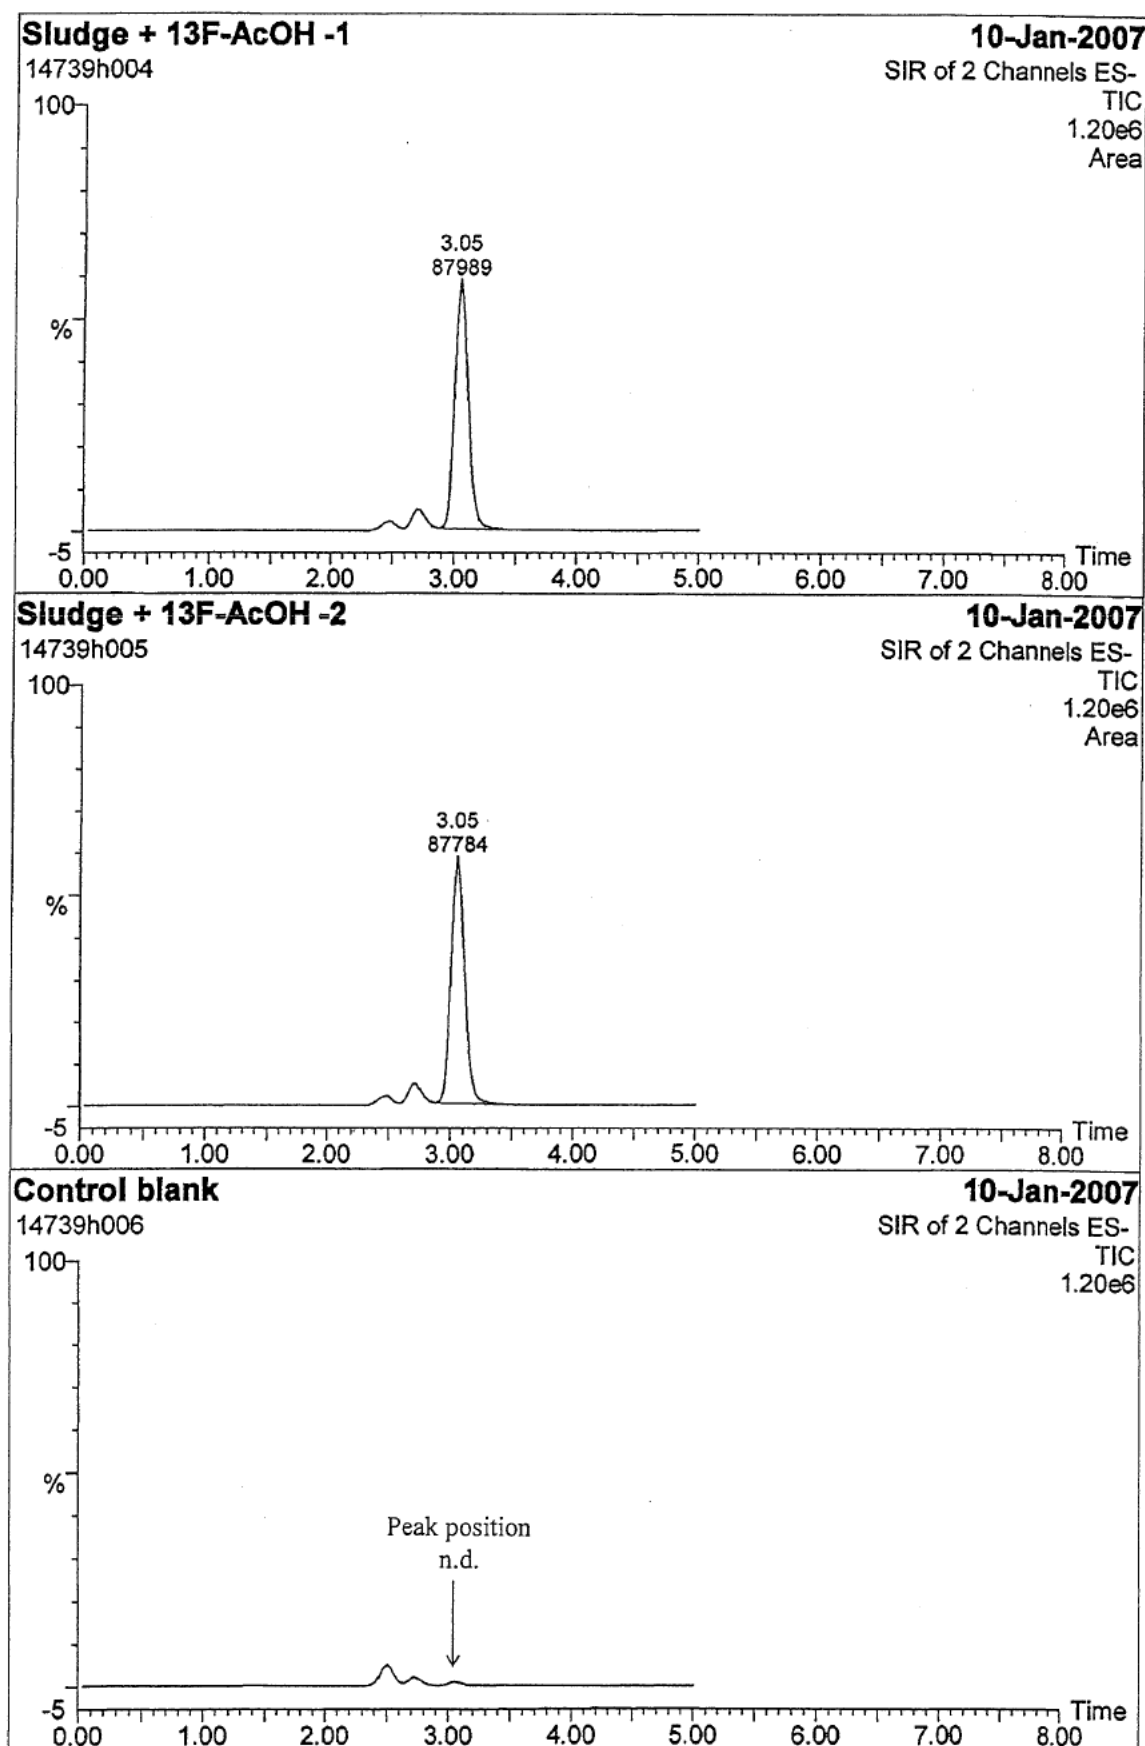


Fig. 8 - 2 Total ion chromatograms of LC-MS analysis for recovery test (13F-AcOH).

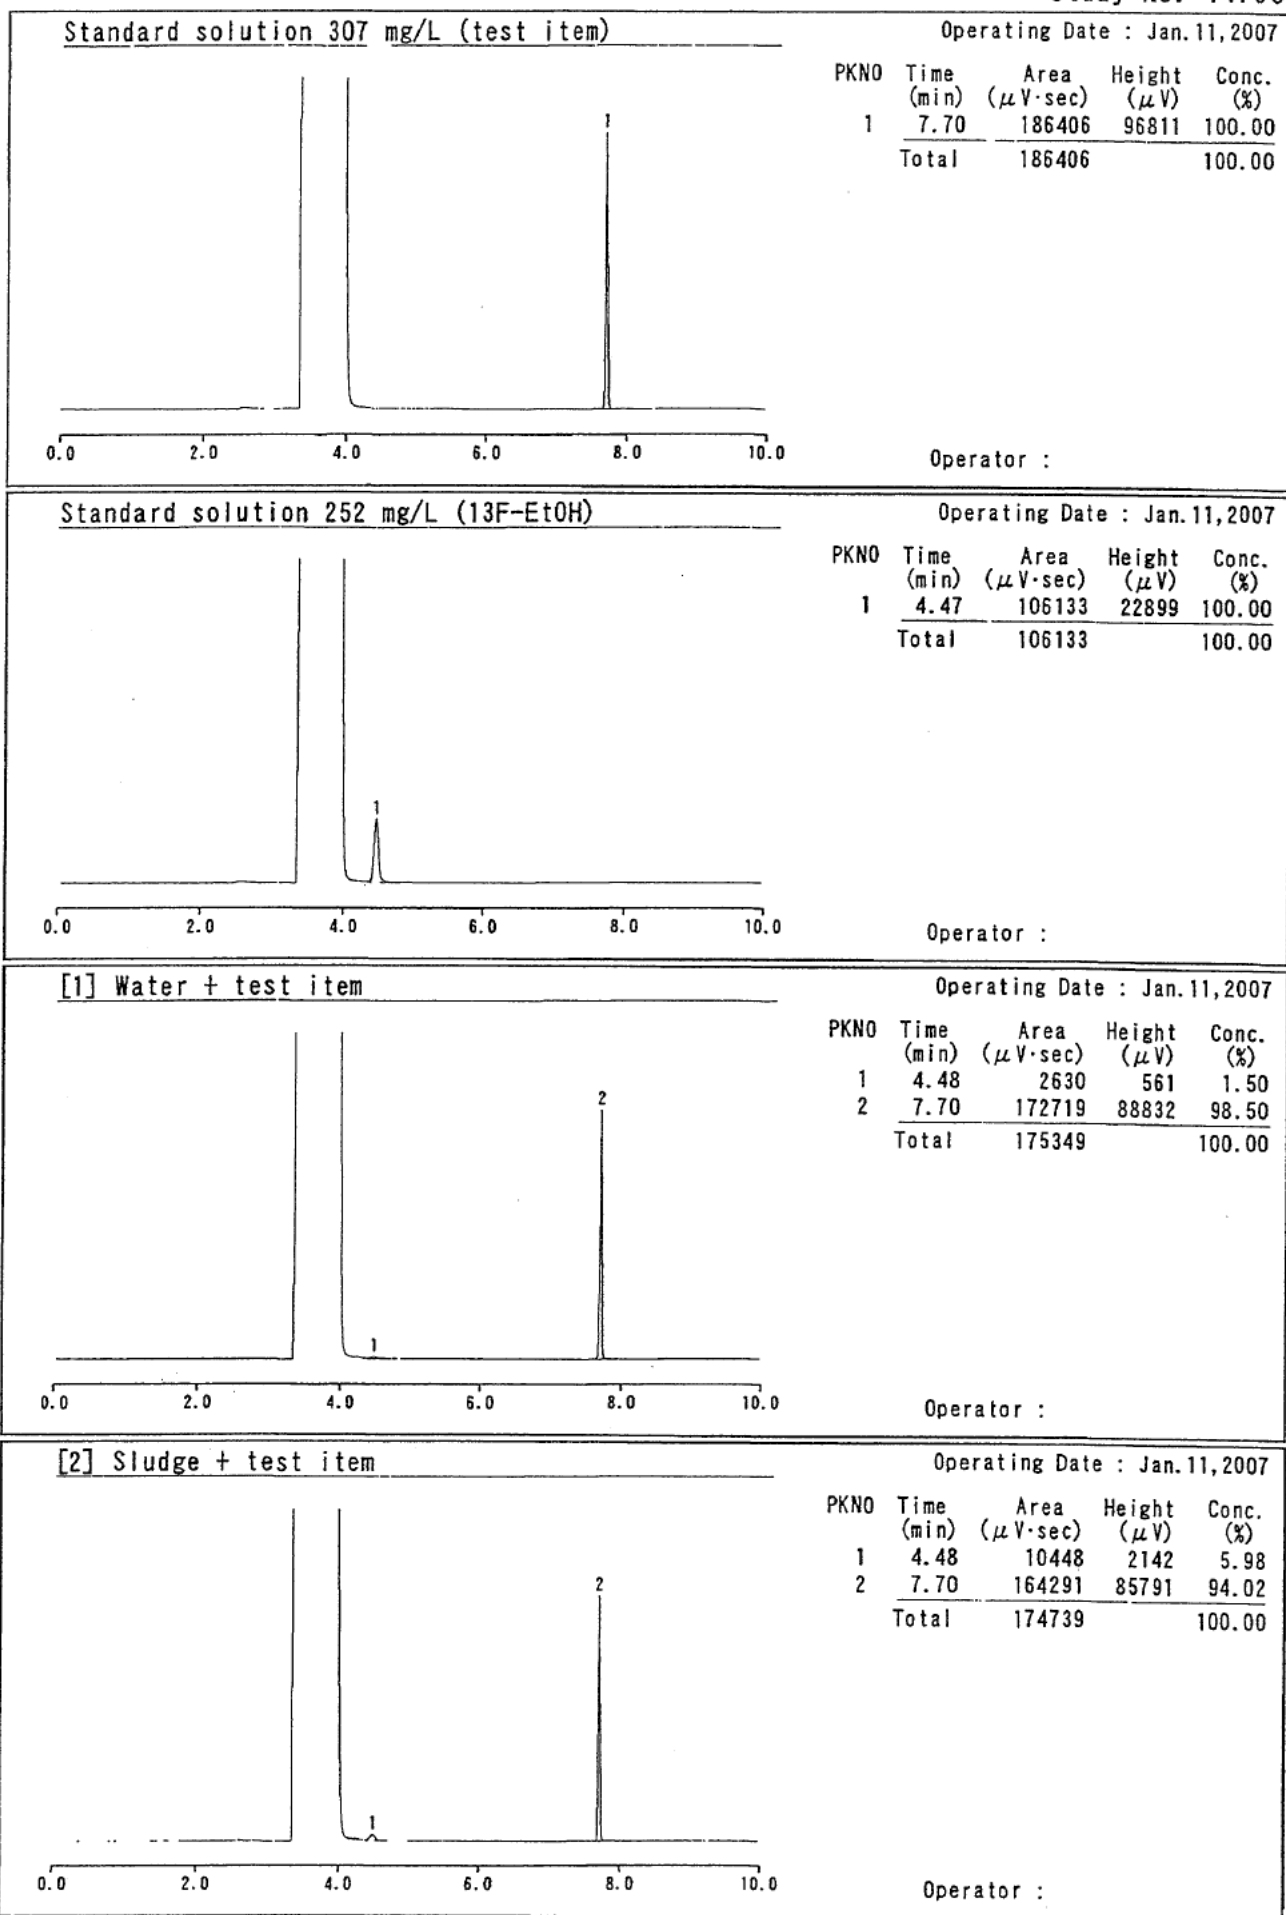


Fig.9 - 1

Chromatograms of GC analysis for test solution
(test item and 13F-EtOH).

Date : Jan.11,2007 Name : _____

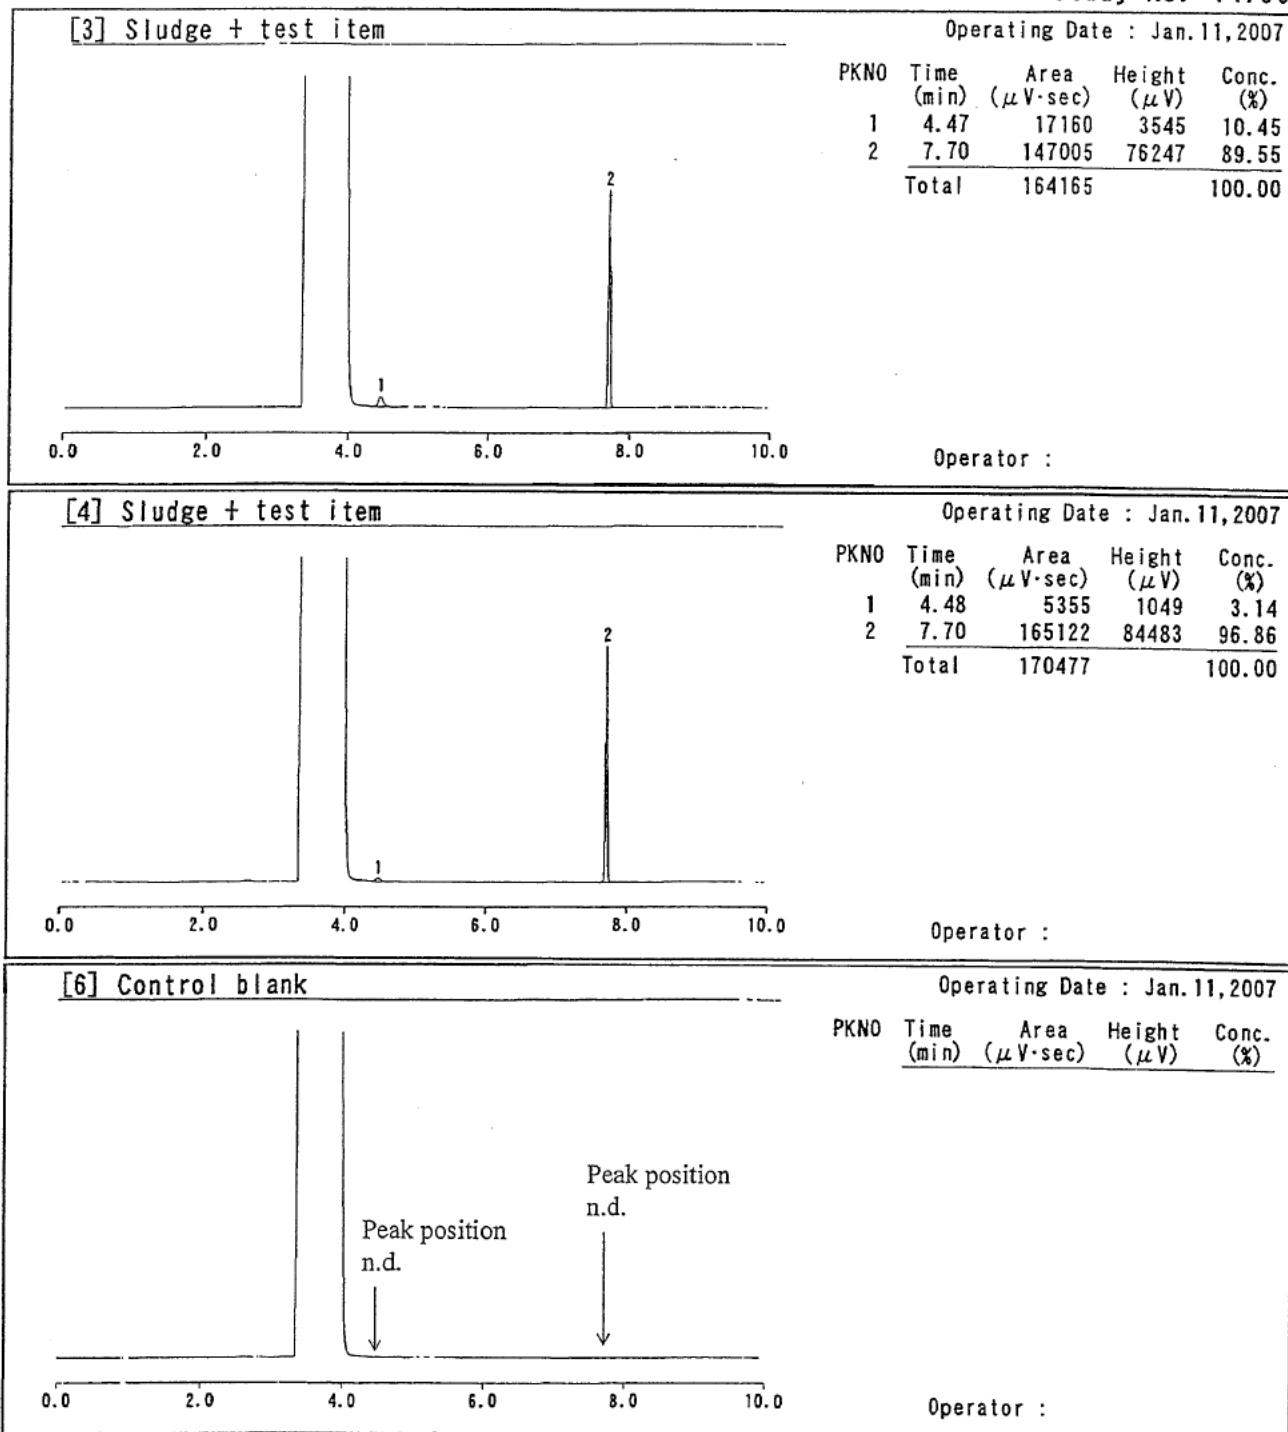


Fig.9 - 2

Chromatograms of GC analysis for test solution
(test item and 13F-EtOH).

Date : Jan.11,2007 Name : _____

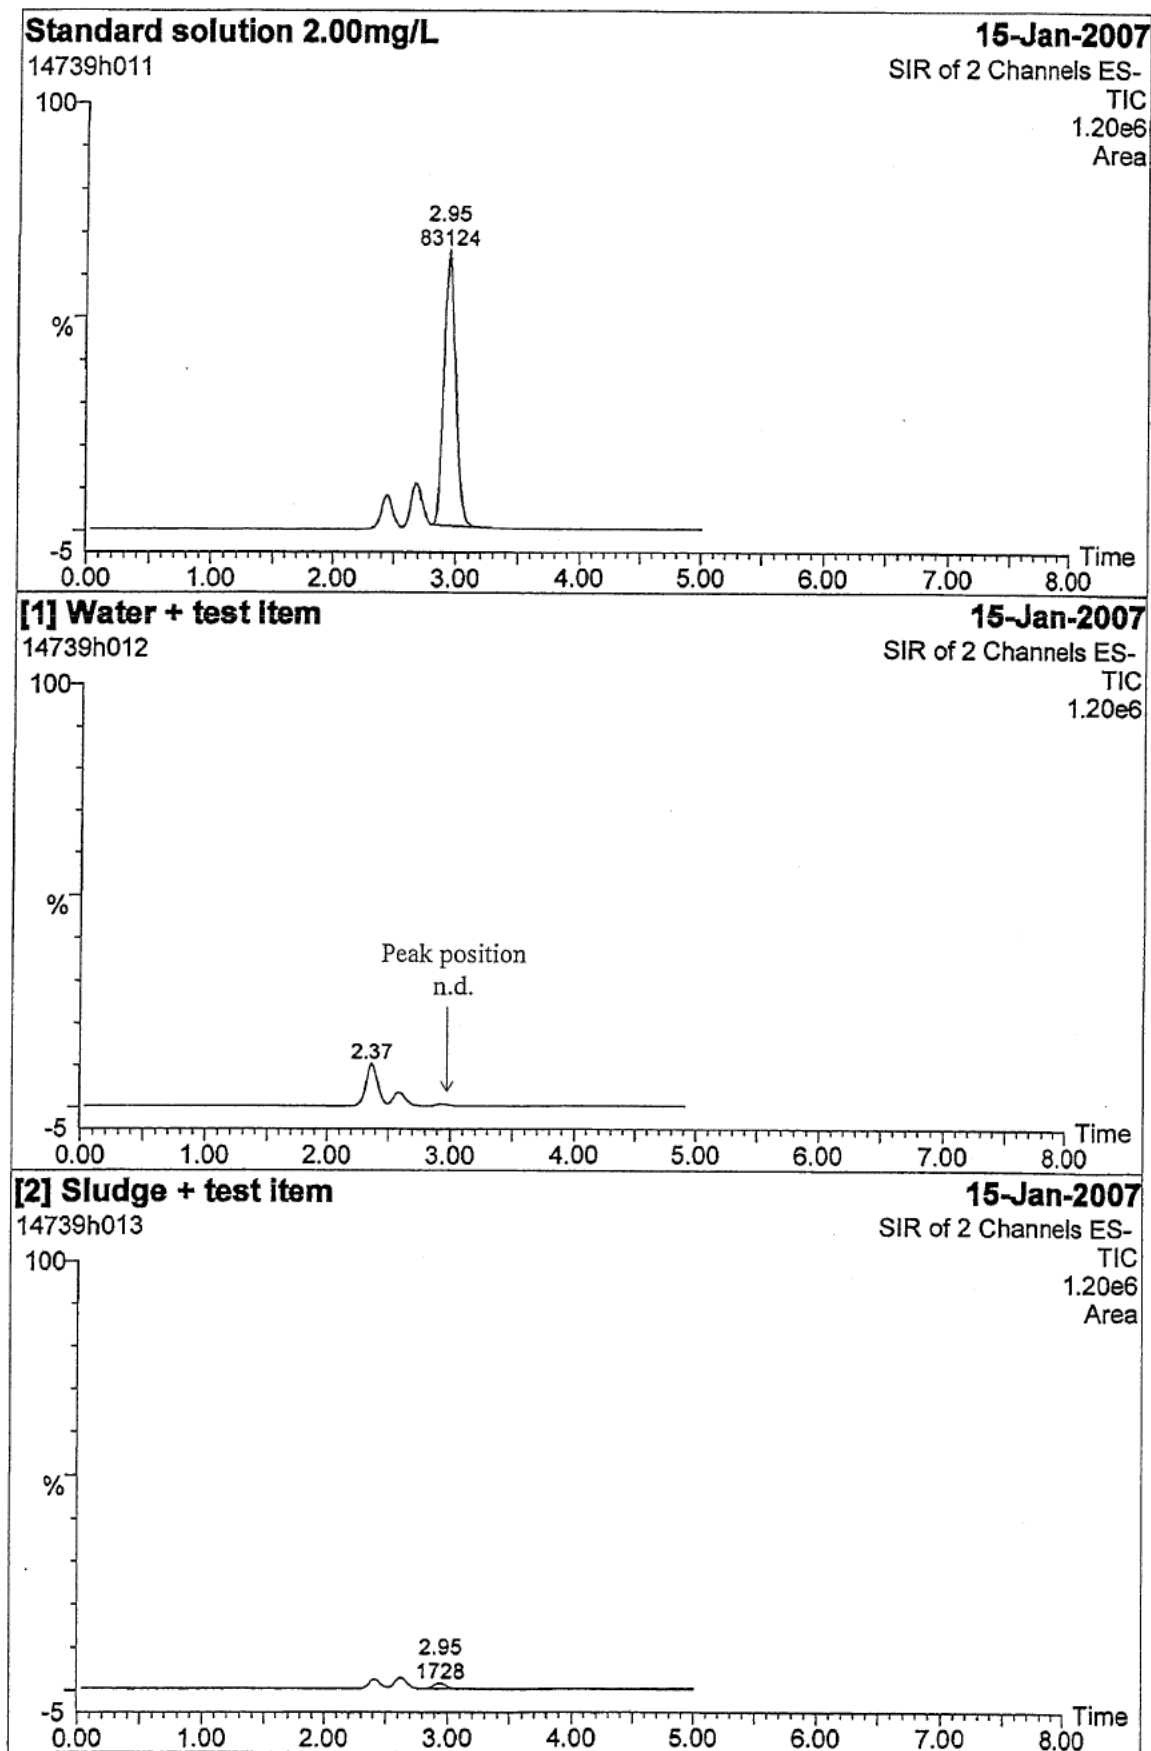


Fig. 10 - 1 Total ion chromatograms of LC-MS analysis for test solution (13F-AcOH).

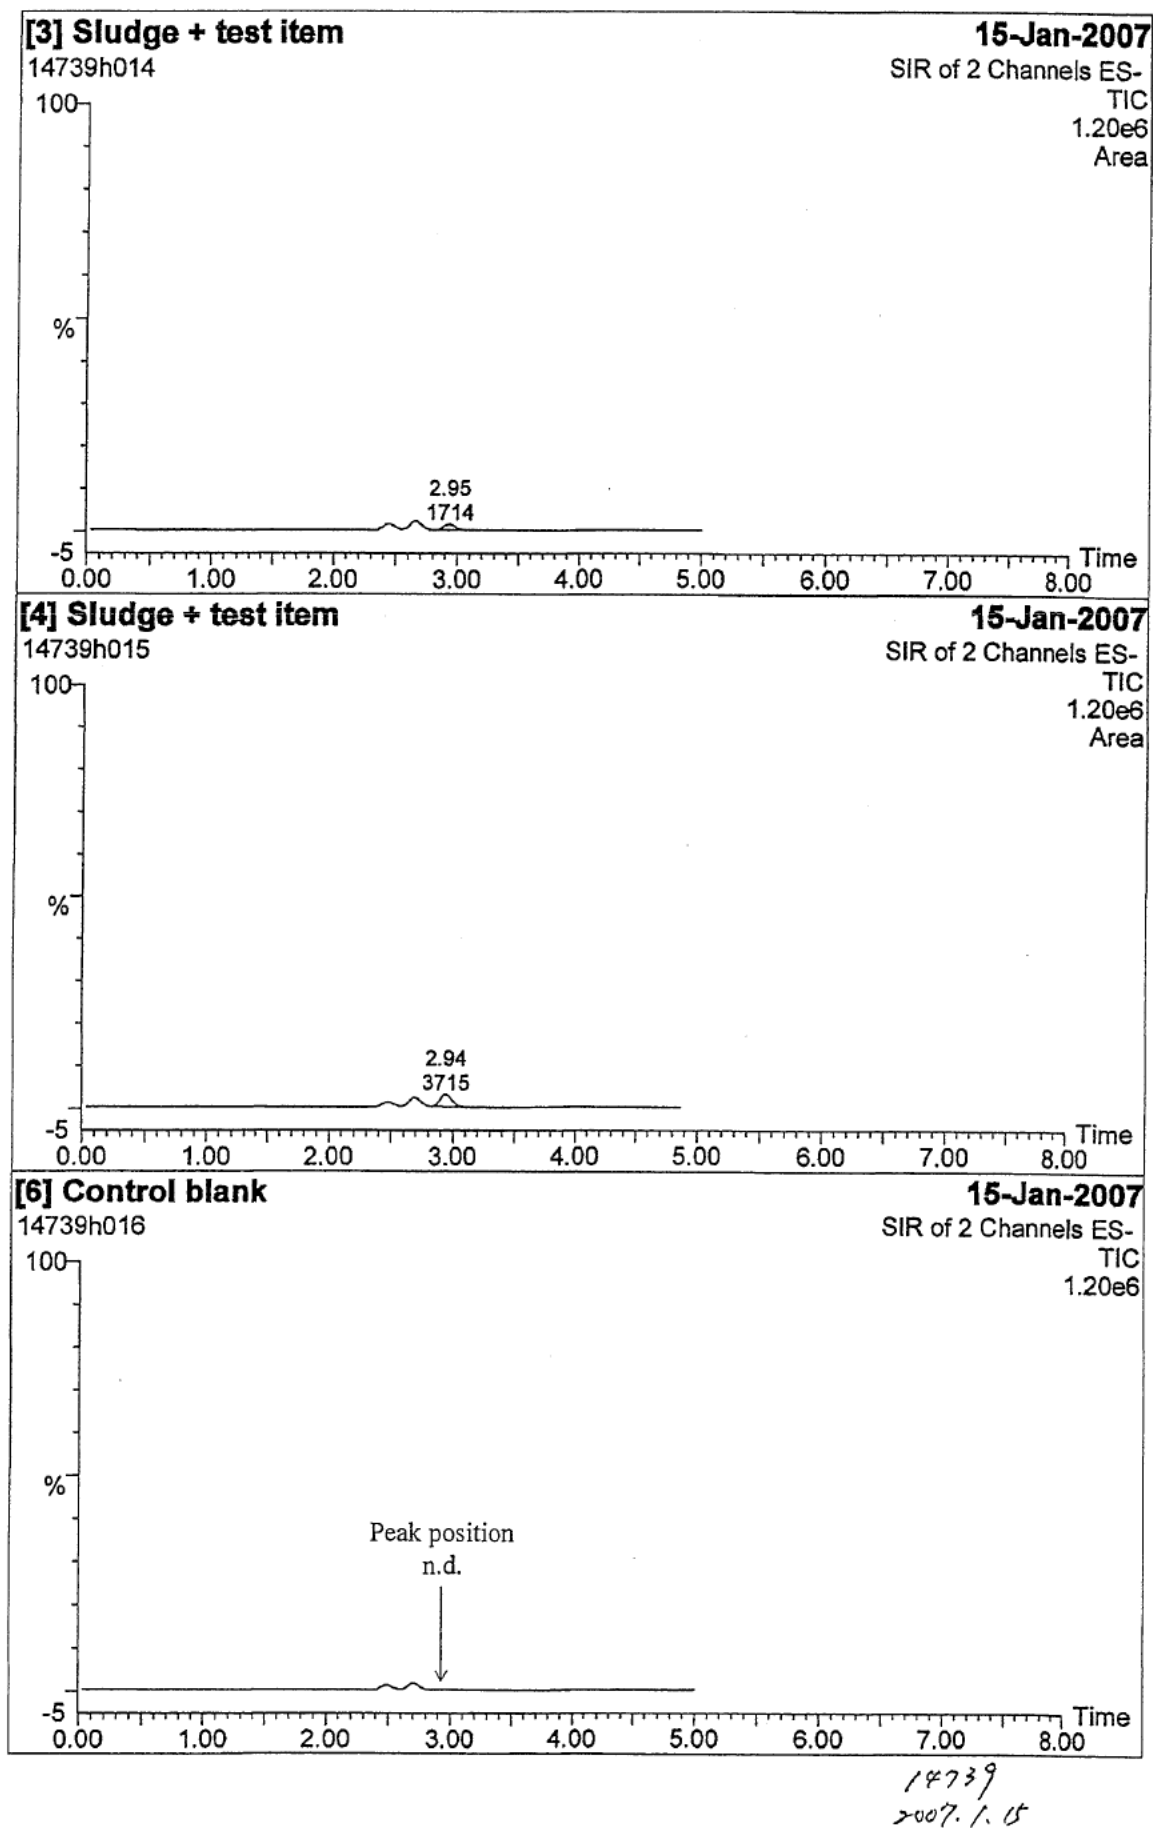


Fig. 10 - 2 Total ion chromatograms of LC-MS analysis for test solution (13F-AcOH).


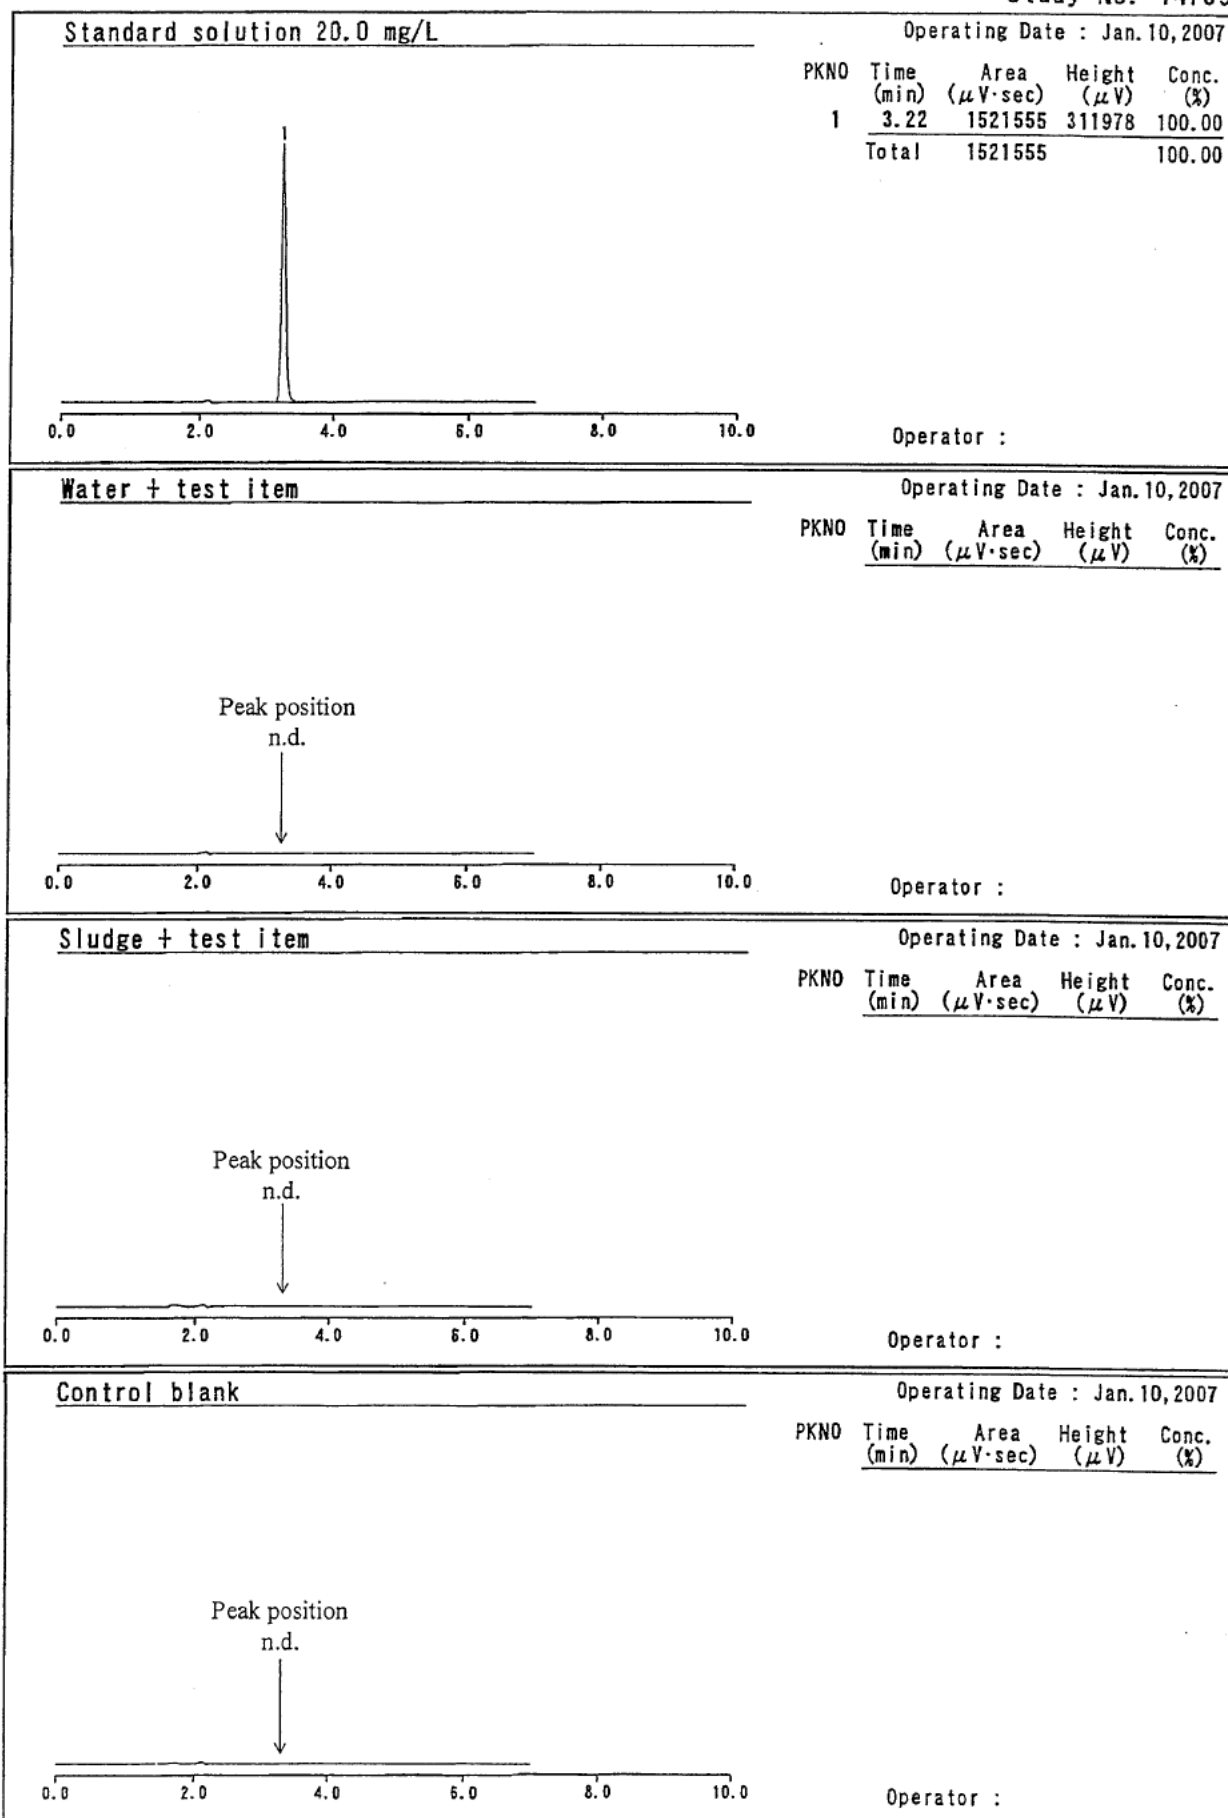


Fig. 11 Chromatograms of HPLC analysis for test solution for analysis of methacrylic acid (methacrylic acid).

Date : Jan.31,2007 Name :

StudyNo.	14739	Wavelength	190.00 - 340.00
Date	Nov. 21, 2006	Scale Limit	1.3000 - -0.1000
Sample	Methacrylic acid	Slit Width	(UV) 2.0nm
Solvent	Purified water	Scan Speed	200nm/min
Reference	-	Sampling Pitch	0.200000
Cell	10mm x 10mm, quartz	Analyst	
Instrument	JASCO	Note	10.0 mg/L
Photometric Mode	Abs		

Chemicals Evaluation and Research Institute, Japan Kurume Laboratory

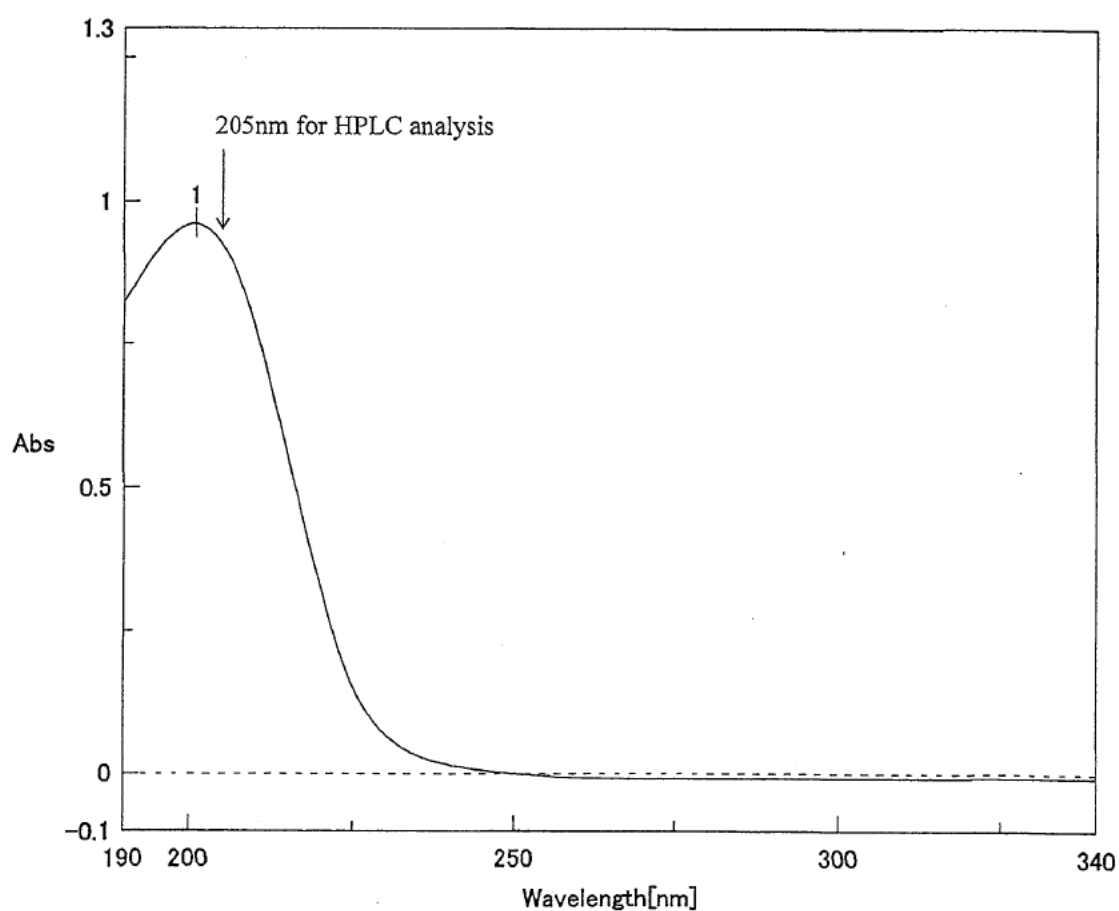

Peak List

1: 201.00 (0.9600)

Fig. 12 UV spectrum of methacrylic acid.

Analytical conditionsInstrument MS : Waters ZMD, LC : Waters Alliance2690Sample 30.0mg/L 13F-AcOH solution

LC Conditions

Inlet system ColumnColumn L-column ODS Column size 15 cm x 2.1 mm I.D.Column temp. 40°CEluent A (80%) : Acetonitrile / formic acid (500/0.25 V/V)B (20%) : Water / formic acid (500/0.25 V/V)Flow rate 0.2 mL/minSample size 2 μ L (Solvent Acetonitrile)

MS Conditions

Ionization mode ESI Detection mode NegativeFunction SCANMass range (m/z) 200 - 1000Probe Capillary 3.0 kV Desolvation temp. 350 °C Desolvation gas 400 L/hrSource Cone 20 V, Extractor 2 V, RF Lens 0.2 VSource block temp. 120 °COperator

Kurume Laboratory, Chemicals Evaluation and Research Institute, Japan

Fig. 13 - 1 Mass spectrum of 13F-AcOH.

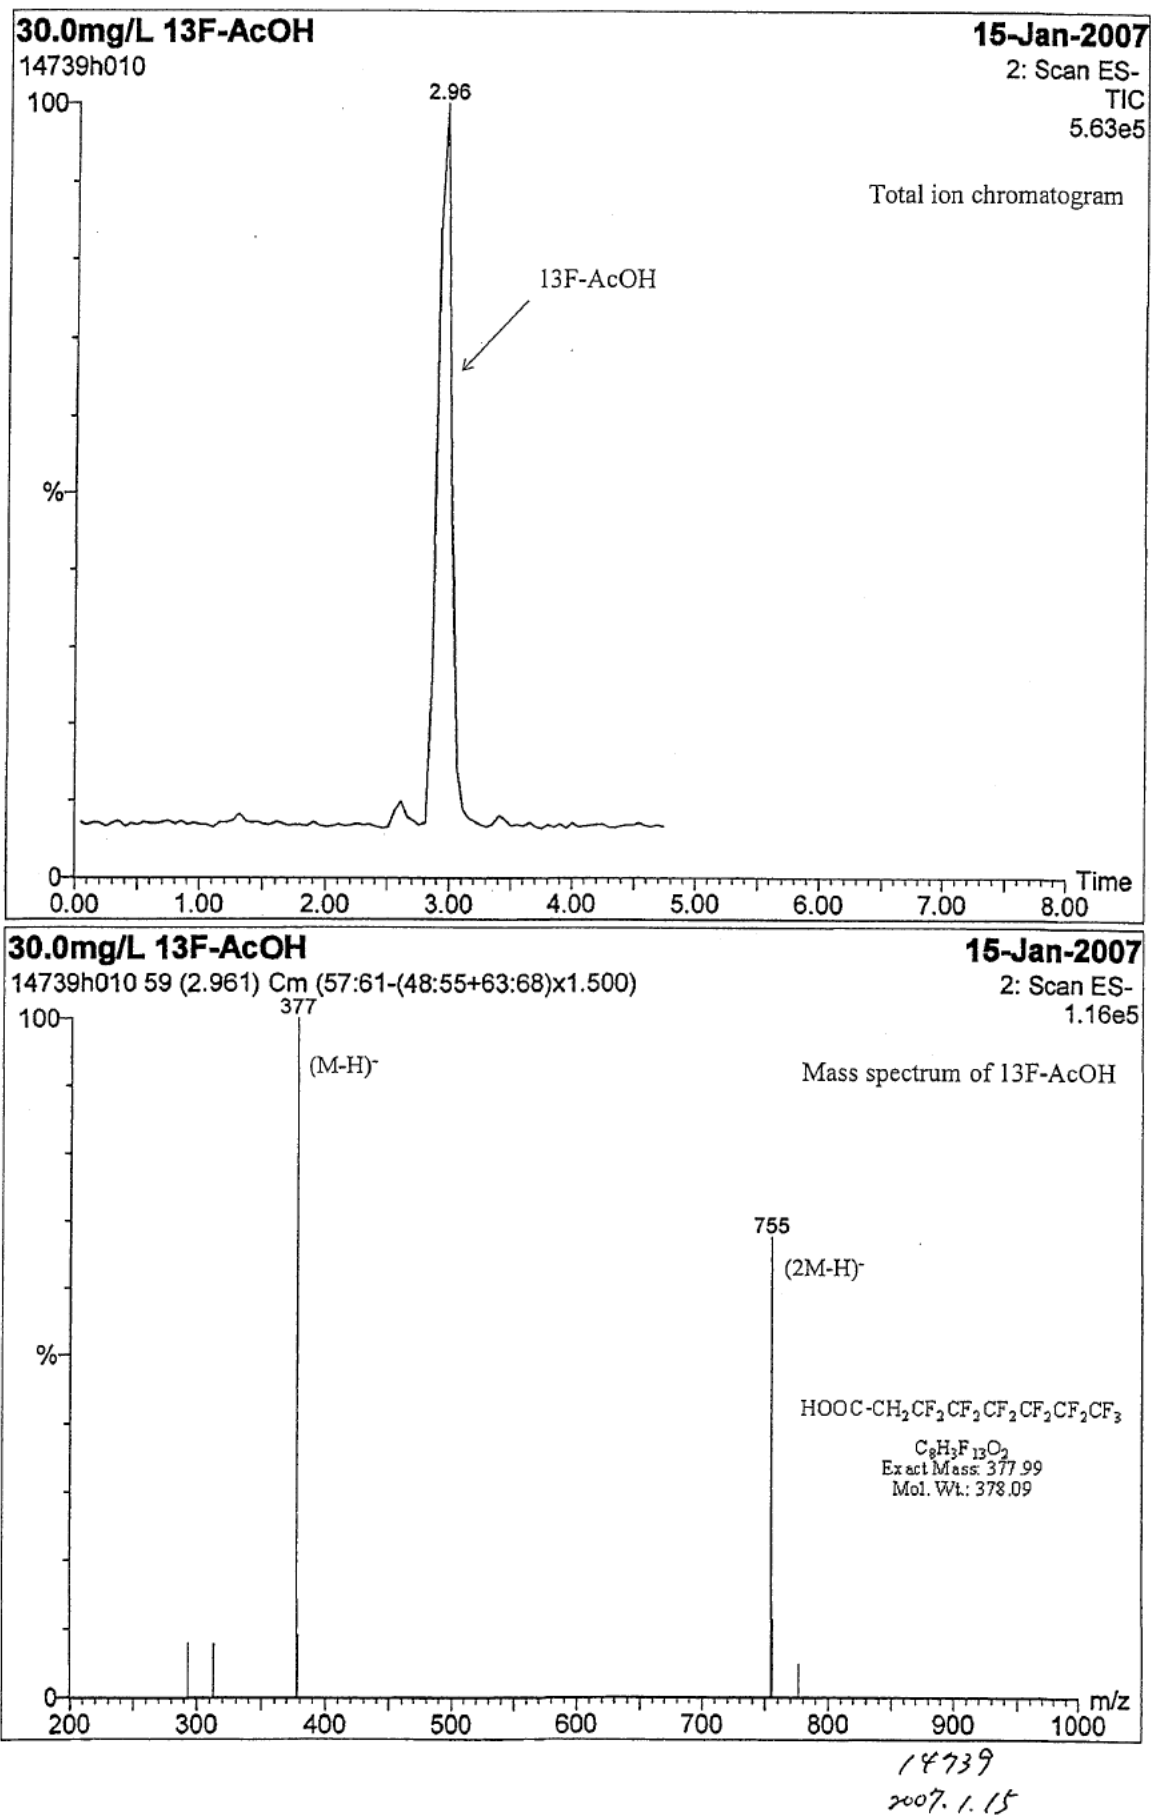


Fig. 13 - 2 Mass spectrum of 13F-AcOH.



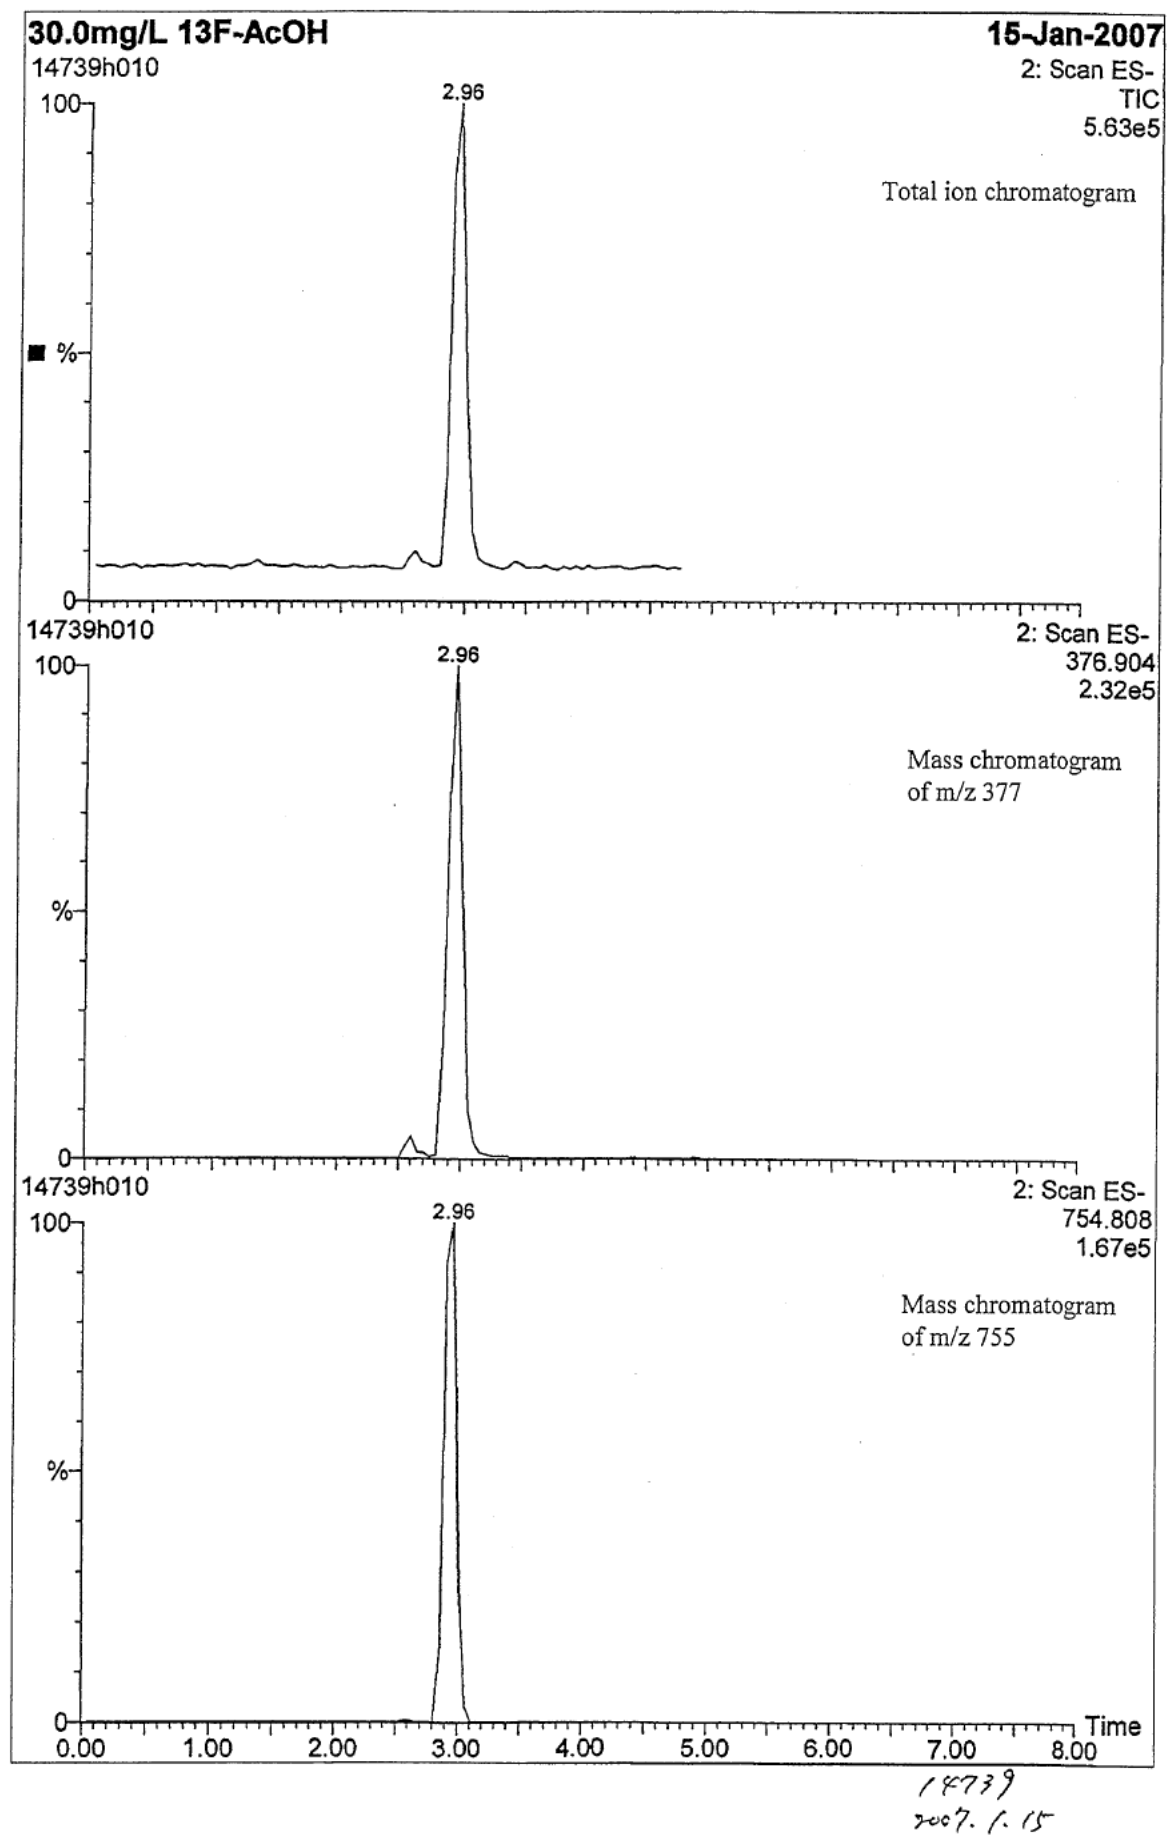


Fig. 13 - 3 Mass spectrum of 13F-AcOH.

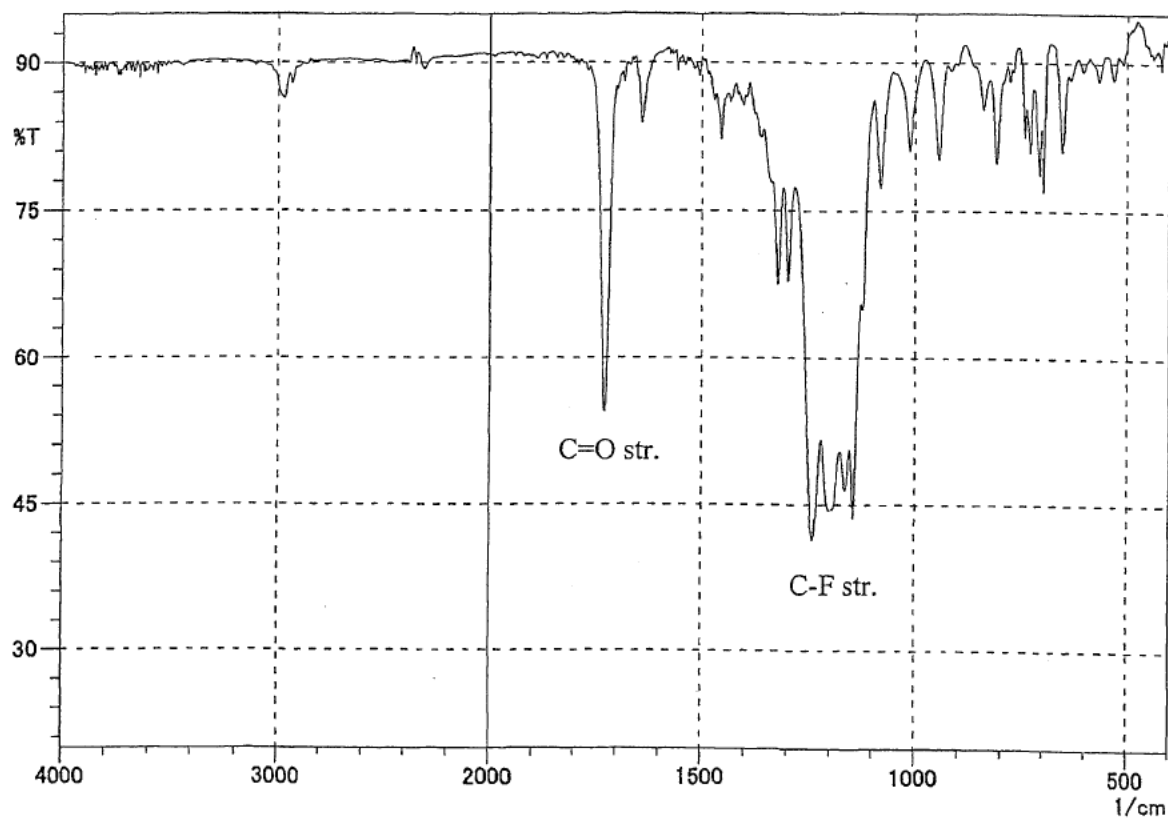


Instrument : Shimadzu IRPrestige-21
Study No. : 14739
Sample : Test item
Method : Neat
Date : November 15, 2006
Name :

Fig.14 - 1 IR spectrum of test item measured before experimental start.

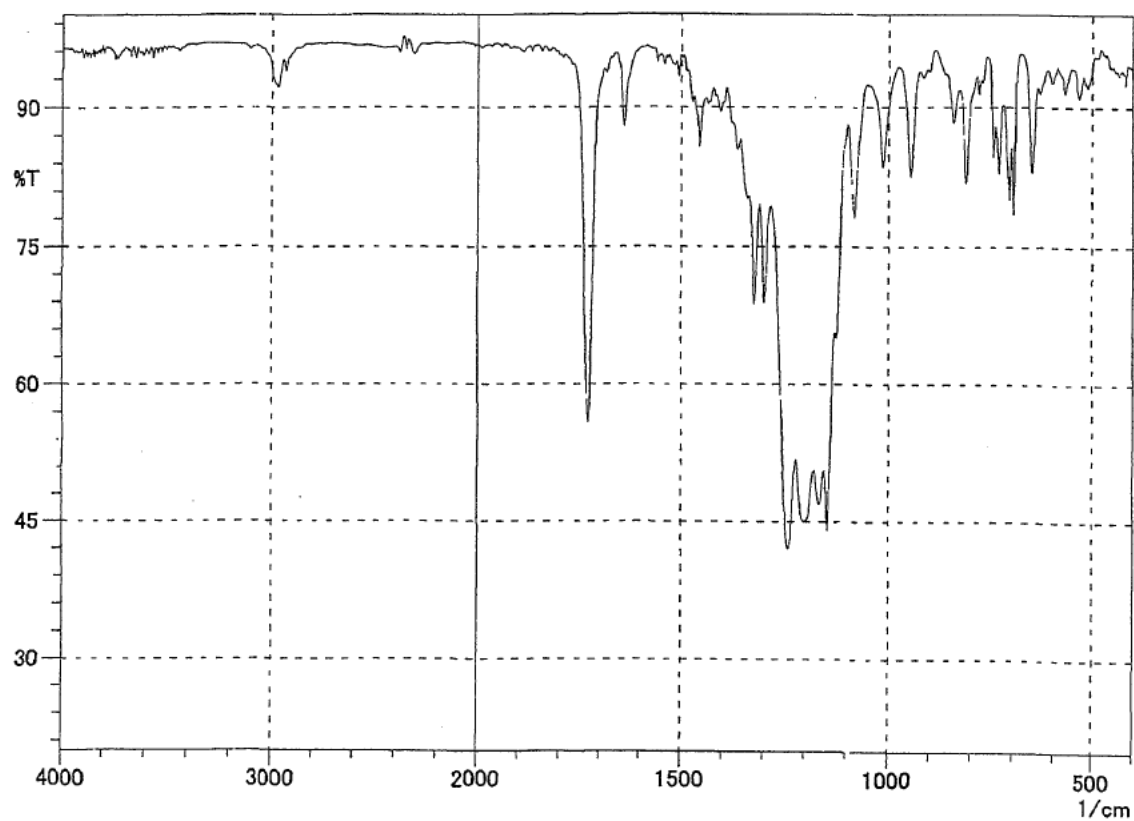

Instrument : Shimadzu IRPrestige-21
Study No. : 14739
Sample : Test item
Method : Neat
Date : January 18, 2007
Name :

Fig.14 - 2 IR spectrum of test item measured after experimental completion.

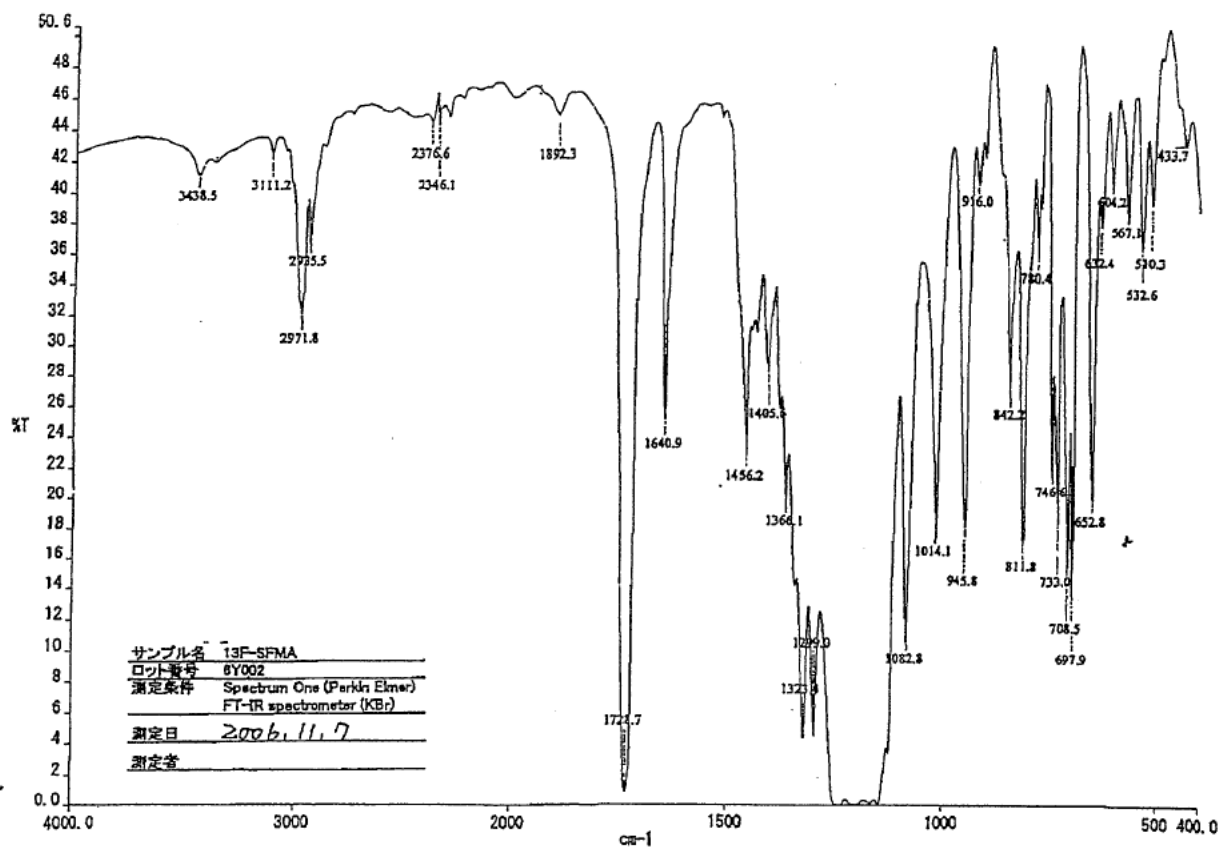


c:\psi_data\spectra\dk5545.sp - 13F-SFMA (Lot. 6Y002)

別紙②

Reference 3 IR spectrum supplied by sponsor.

Standard solution 20.0 mg/L

Operating Date : Jan. 15, 2007

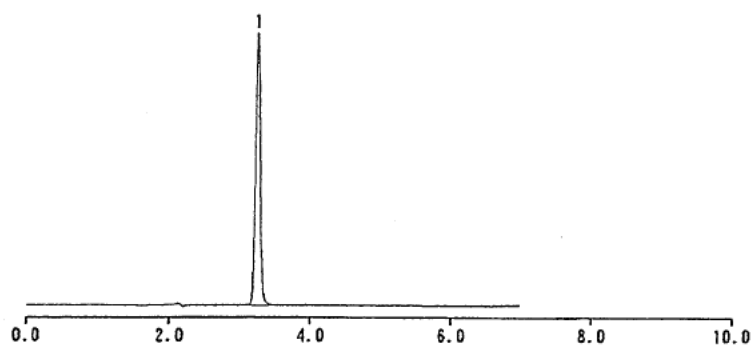


PKNO	Time (min)	Area ($\mu\text{V}\cdot\text{sec}$)	Height (μV)	Conc. (%)
1	3.22	1518705	311896	100.00
Total		1518705		100.00

Operator :

Water + test item

Operating Date : Jan. 15, 2007



PKNO	Time (min)	Area ($\mu\text{V}\cdot\text{sec}$)	Height (μV)	Conc. (%)
1	3.22	225650	46522	100.00
Total		225650		100.00

Operator :

Sludge + test item

Operating Date : Jan. 15, 2007




PKNO	Time (min)	Area ($\mu\text{V}\cdot\text{sec}$)	Height (μV)	Conc. (%)
1	3.22	140937	28964	100.00
Total		140937		100.00

Operator :

Control blank

Operating Date : Jan. 15, 2007

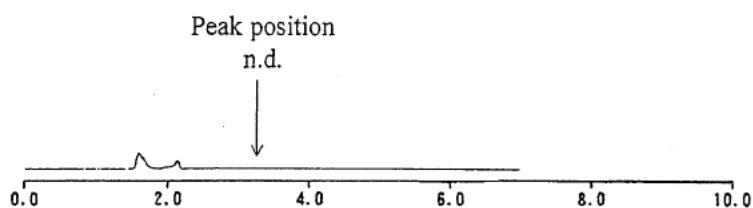

PKNO	Time (min)	Area ($\mu\text{V}\cdot\text{sec}$)	Height (μV)	Conc. (%)
------	------------	---------------------------------------	--------------------------	-----------

Operator :


Reference 4 Chromatograms of HPLC analysis for CO₂ absorbent (methacrylic acid, test solution for analysis of methacrylic acid).

Date : Jan. 15, 2007 Name : _____

Standard solution 20.0 mg/L

Operating Date : Jan.15,2007

PKNO	Time (min)	Area (μ V·sec)	Height (μ V)	Conc. (%)
1	3.23	1523373	305754	100.00
Total		1523373		100.00

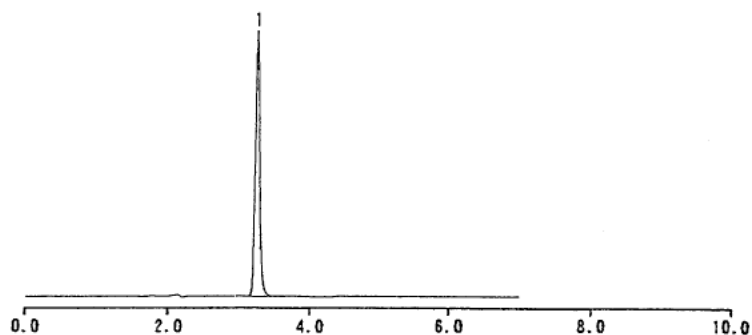


Operator :

[1] Water + test item

Operating Date : Jan.15,2007

PKNO	Time (min)	Area (μ V·sec)	Height (μ V)	Conc. (%)
1	3.22	275549	56614	100.00
Total		275549		100.00

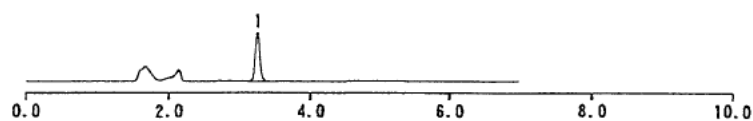


Operator :

[2] Sludge + test item

Operating Date : Jan.15,2007

PKNO	Time (min)	Area (μ V·sec)	Height (μ V)	Conc. (%)
1	3.22	103843	21345	100.00
Total		103843		100.00



Operator :

Reference 5 - 1


Chromatograms of HPLC analysis for CO₂ absorbent
(methacrylic acid).

Date : Jan.15,2007 Name : _____

[3] Sludge + test item

Operating Date : Jan. 15, 2007

PKNO	Time (min)	Area (μ V-sec)	Height (μ V)	Conc. (%)
1	3.22	165511	34079	100.00
Total		165511		100.00




Operator :

[4] Sludge + test item

Operating Date : Jan. 15, 2007

PKNO	Time (min)	Area (μ V-sec)	Height (μ V)	Conc. (%)
1	3.22	108086	22162	100.00
Total		108086		100.00




Operator :

[6] Control blank

Operating Date : Jan. 15, 2007

PKNO	Time (min)	Area (μ V-sec)	Height (μ V)	Conc. (%)
------	---------------	------------------------	----------------------	--------------

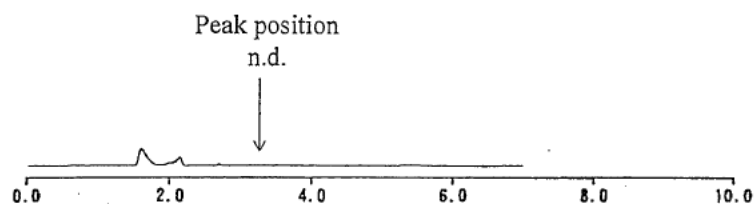

Operator :

Reference 5 - 2

Chromatograms of HPLC analysis for CO₂ absorbent
(methacrylic acid).

Date : Jan. 15, 2007 Name : _____

確認番号 001

基準適合試験施設確認書

財団法人化学物質評価研究機構
理事長 近藤 雅臣 殿

化学物質の審査及び製造等の規制に関する法律に係る試験施設に関する基準適合確認実施要領に基づき、下記試験施設については、新規化学物質に係る試験並びに第一種監視化学物質及び第二種監視化学物質に係る有害性の調査の項目等を定める省令第4条に規定する試験施設に関する基準に適合していることを確認します。

なお、確認の有効期間は、本確認書の交付日から起算して3年間とします。

平成16年12月22日

経済産業省製造産業局長 石毛 博行



記

試験施設の名称	財団法人化学物質評価研究機構 久留米事業所
試験施設の所在地	福岡県久留米市宮ノ陣三丁目2番7号
試験項目	分解度試験、濃縮度試験及び分配係数試験